
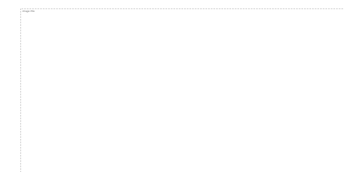


Instrument AV700
EX435

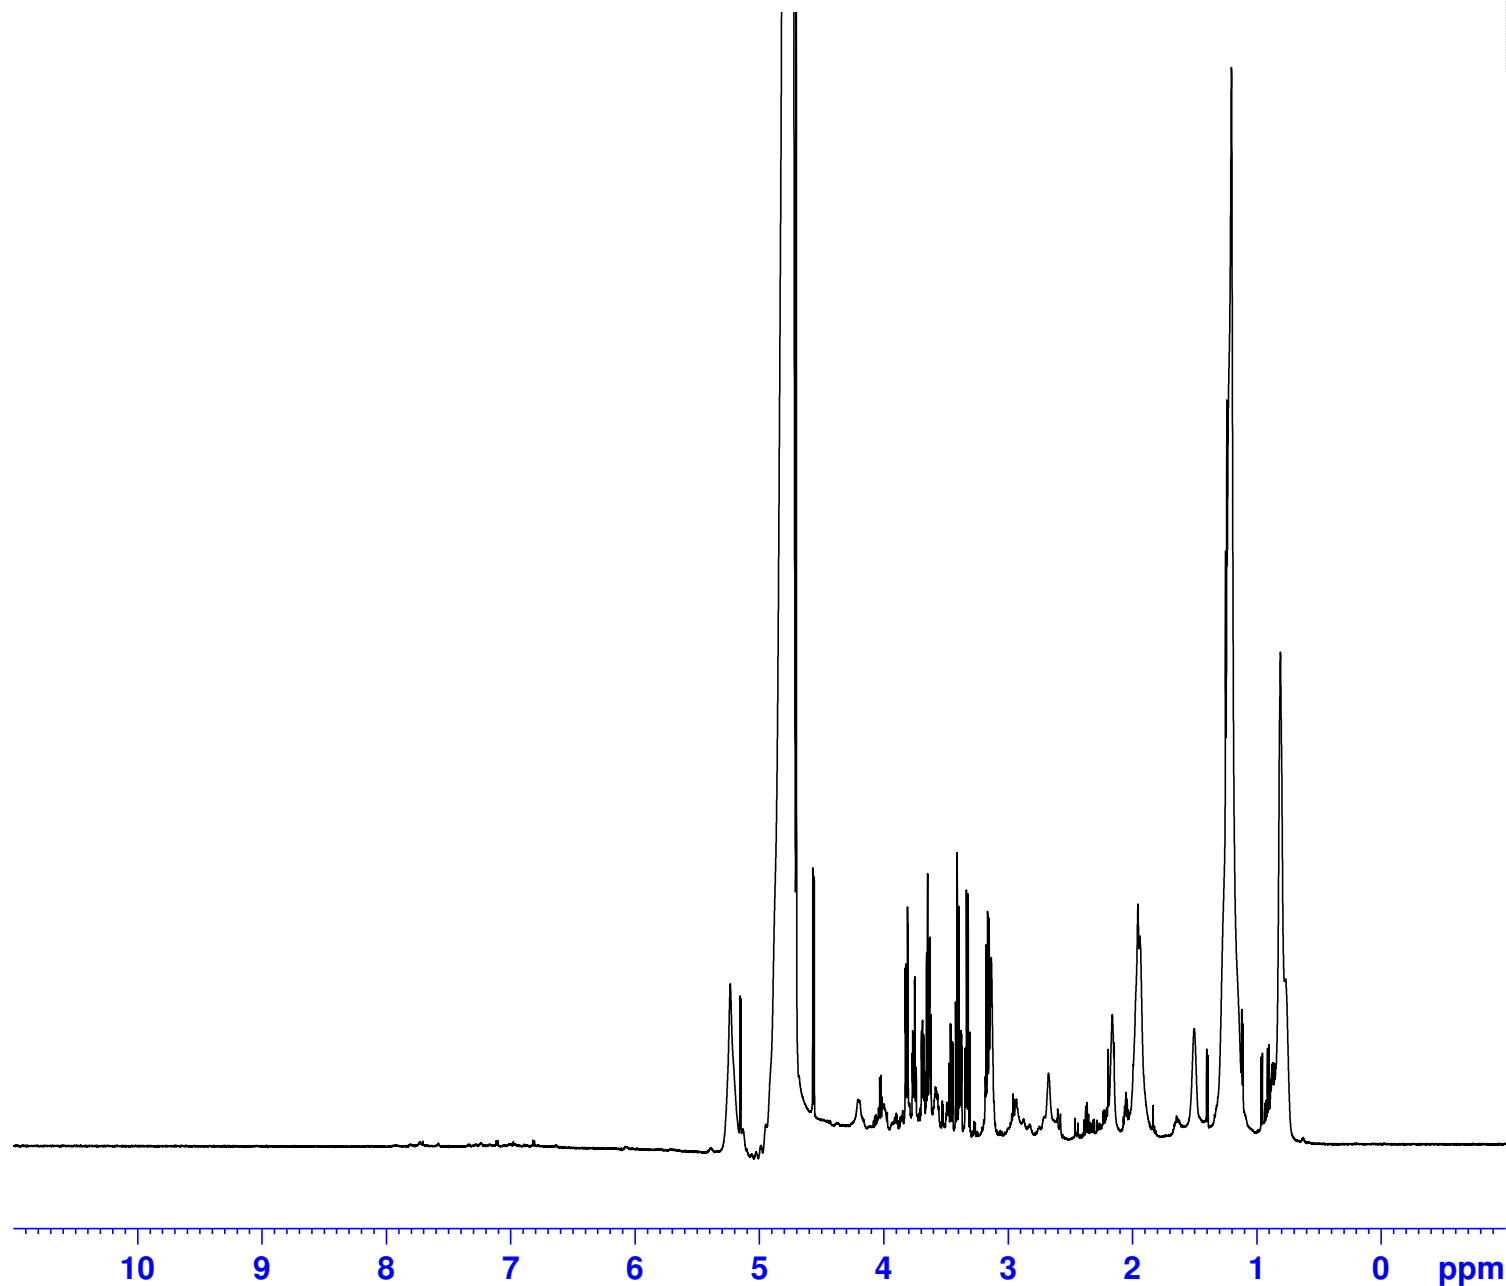

Current Data Parameters
NAME 20230126_TK_MS_extreme_phenotypes
EXPNO 2435
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230129
Time 13.00 h
INSTRUM av700
PROBHD Z44908_0059 (C
PULPROG cpmgpr_project
TD 32768
SOLVENT Serum
NS 32
DS 8
SWH 11194.030 Hz
FIDRES 0.683229 Hz
AQ 1.4636374 sec
RG 32
DW 44.667 usec
DE 10.51 usec
TE 298.0 K
D1 2.00000000 sec
D12 0.00002000 sec
D20 0.00100000 sec
D21 0.04000000 sec
L4 20
TD0 1
SF01 699.8532935 MHz
NUC1 1H
P1 16.70 usec
P2 33.40 usec
PLW1 5.01189995 W
PLW9 0.00005591 W

F2 - Processing parameters
SI 65536
SF 699.8500000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00