
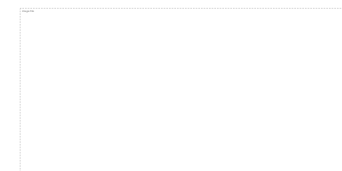


Instrument AVH400
Group HJS
Chemist Suer
h1acqQ.crl DMSO {C:\NMR} hjsgrp 46

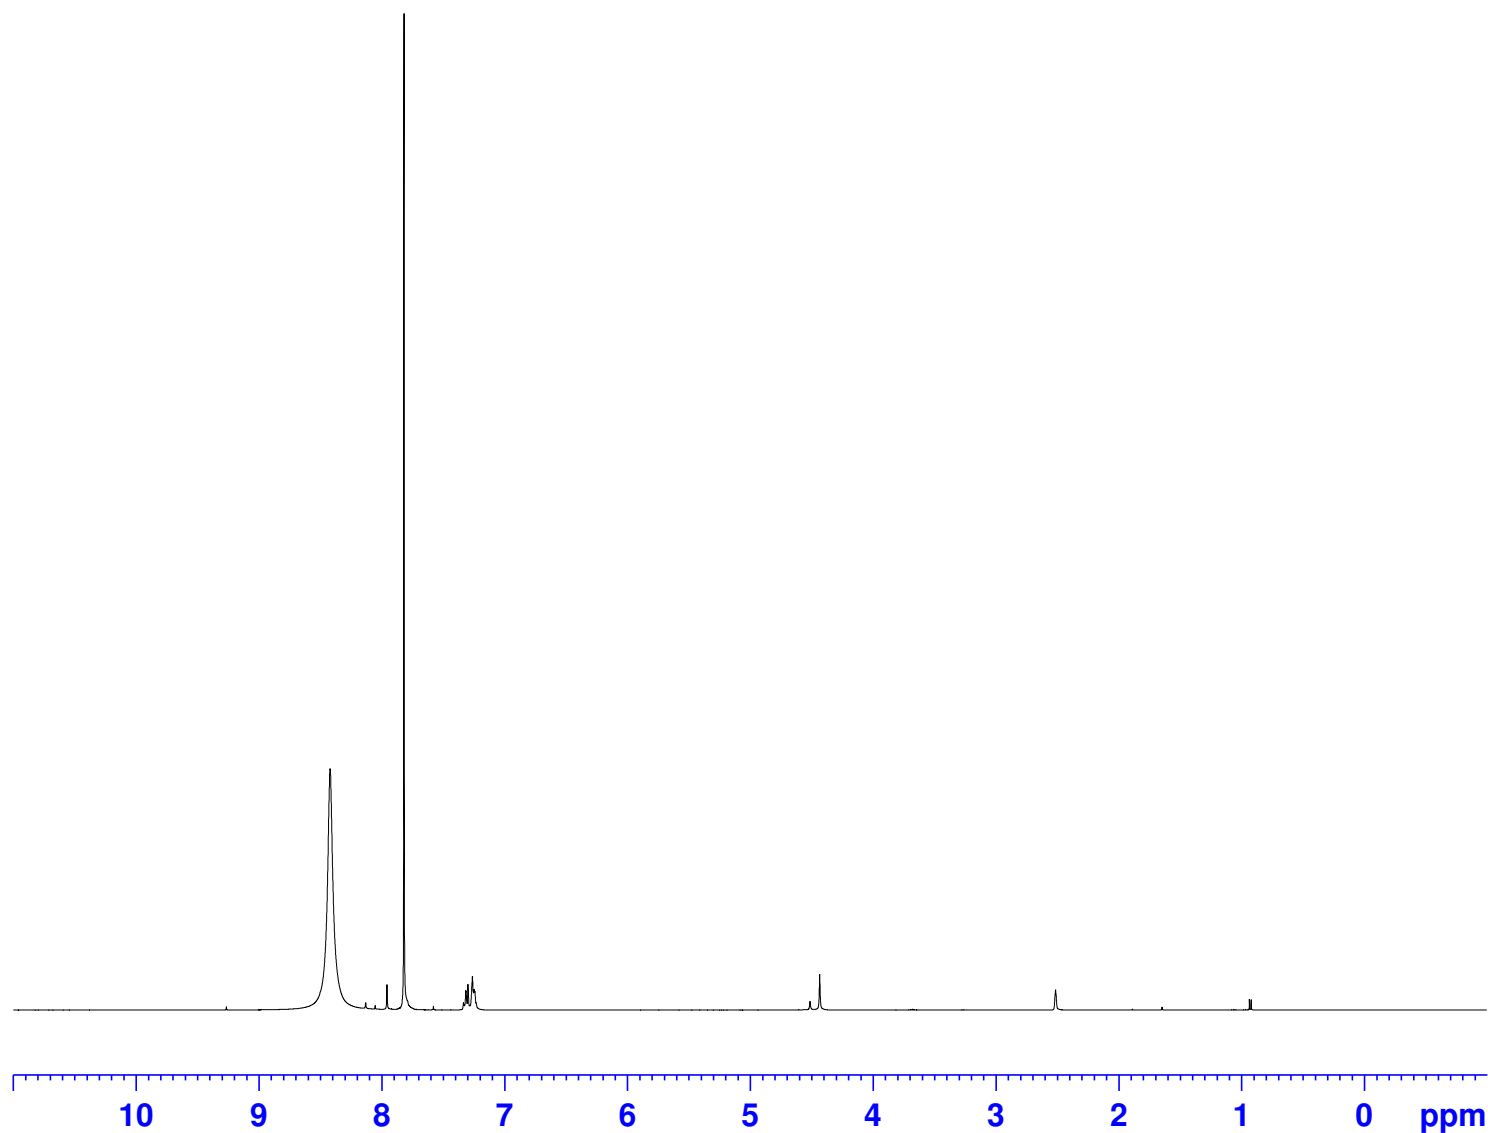

Current Data Parameters
NAME Apr22-2022-46-Cs25Br20 plus 5percent Bza
EXPNO 4
PROCNO 1

F2 - Acquisition Parameters
Date_ 20220422
Time_ 13.06 h
INSTRUM avh400
PROBHD Z108618_0873 (
FULPROG zg
TD 65536
SOLVENT DMSO
NS 4
DS 0
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 24.41
DW 62.400 usec
DE 6.50 usec
TE 298.1 K
D1 25.00000000 sec
TDO 1
SFO1 400.1324008 MHz
NUC1 1H
P1 14.00 usec
PLW1 14.36999989 W

F2 - Processing parameters
SI 32768
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00