
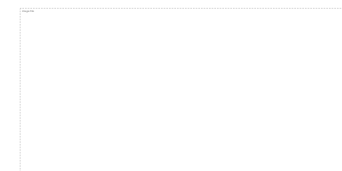


Instrument AVH400  
Group HJS  
Chemist Suer  
h1acqQ.crl DMSO {C:\NMR} hjsgrp 47

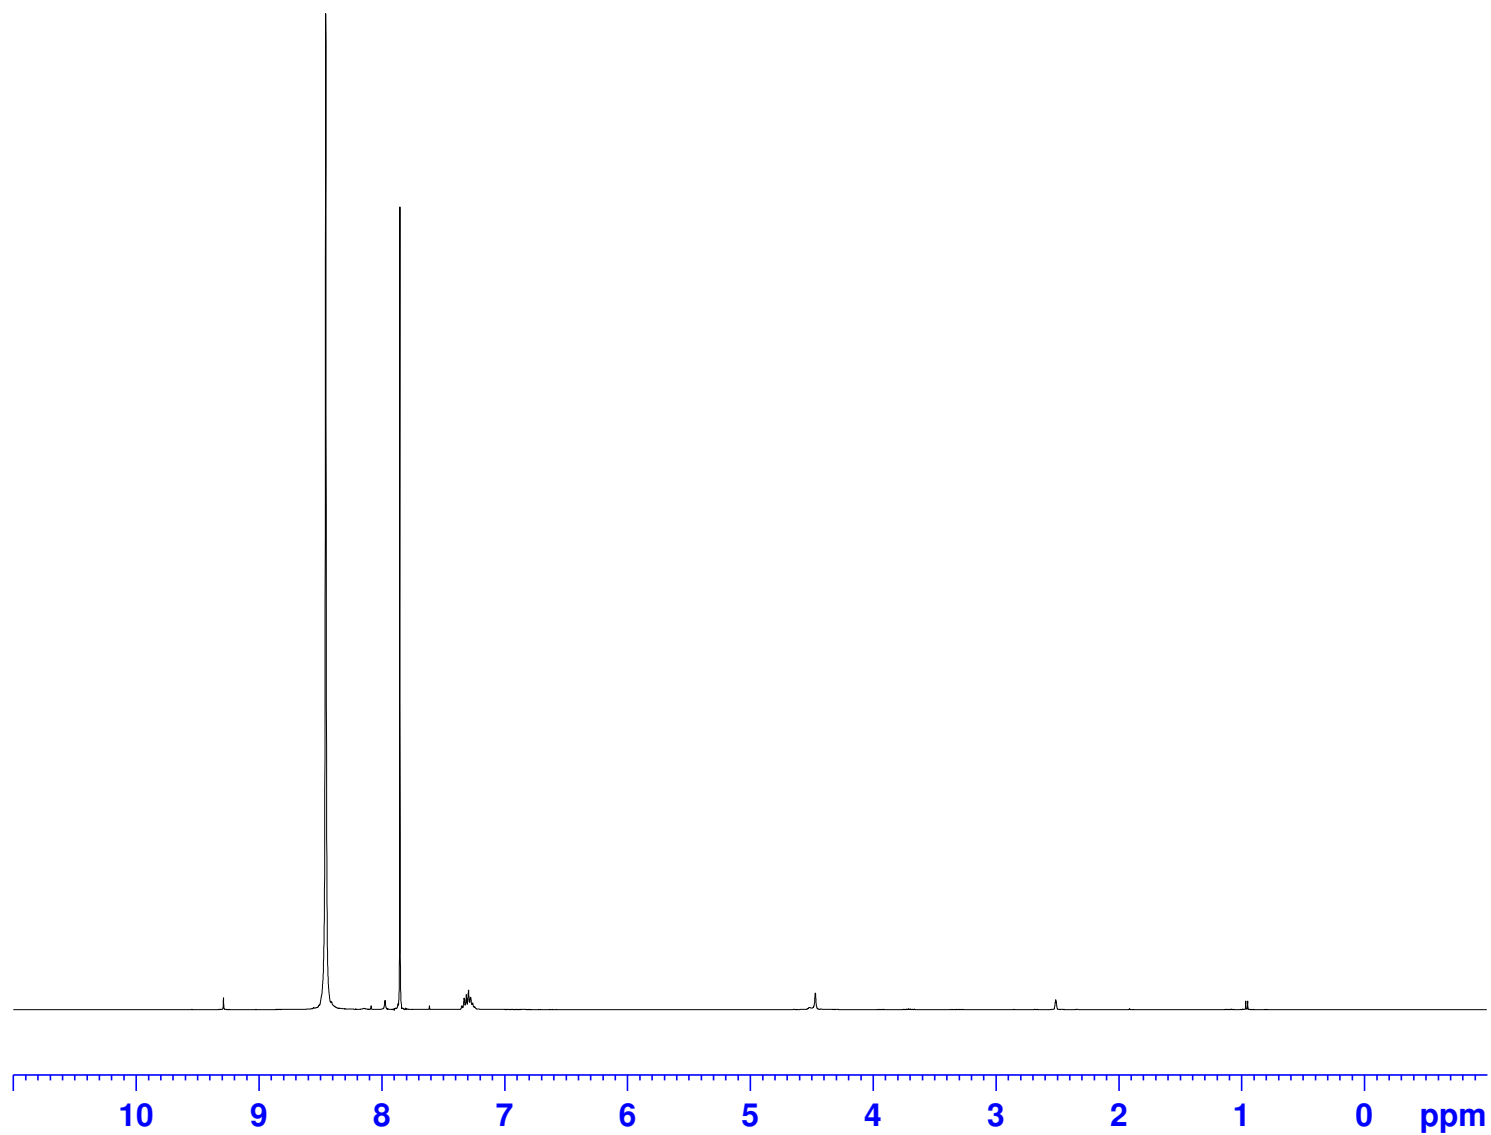

Current Data Parameters  
NAME Apr22-2022-47-FAI plus 5percent Bza  
EXPNO 1  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20220422  
Time 13.13 h  
INSTRUM avh400  
PROBHD Z108618\_0873 (  
PULPROG zg  
TD 65536  
SOLVENT DMSO  
NS 4  
DS 0  
SWH 8012.820 Hz  
FIDRES 0.244532 Hz  
AQ 4.0894465 sec  
RG 15.33  
DW 62.400 usec  
DE 6.50 usec  
TE 298.0 K  
D1 25.00000000 sec  
TD0 1  
SFO1 400.1324008 MHz  
NUC1 1H  
P1 14.00 usec  
PLW1 14.36999989 W

F2 - Processing parameters  
SI 32768  
SF 400.1300000 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00