


Instrument AVH400
Group HJS
Chemist Suer
c13acq_512.crl DMSO {C:\NMR} hjsgrp 1

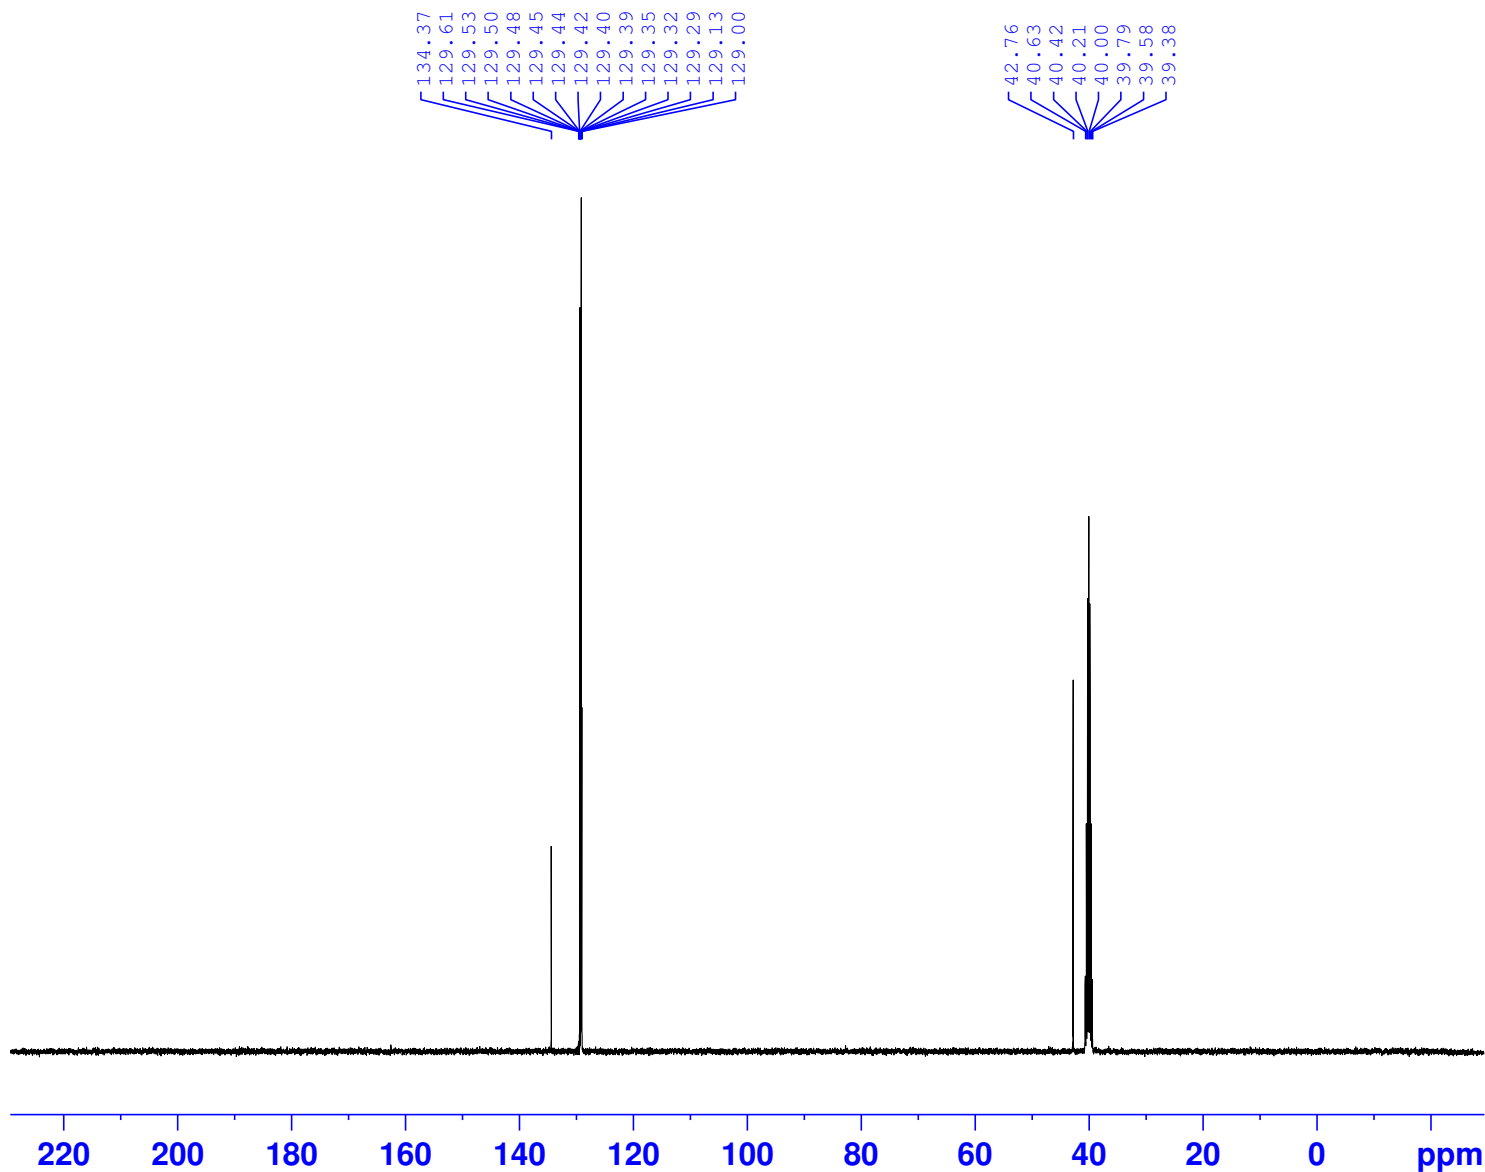

Current Data Parameters
NAME Jul25-2022-1-BzaI
EXPNO 2
PROCNO 1

F2 - Acquisition Parameters
Date_ 20220725
Time 20.55 h
INSTRUM avh400
PROBHD Z116098_0219 (
PULPROG zgpg30
TD 32768
SOLVENT DMSO
NS 512
DS 4
SWH 26041.666 Hz
FIDRES 1.589457 Hz
AQ 0.6291456 sec
RG 197.18
DW 19.200 usec
DE 6.50 usec
TE 296.6 K
D1 1.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 100.6228298 MHz
NUC1 13C
P0 3.67 usec
P1 11.00 usec
PLW1 69.00000000 W
SFO2 400.1316005 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 16.00000000 W
PLW12 0.19753000 W
PLW13 0.09935700 W

F2 - Processing parameters
SI 32768
SF 100.6127685 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40