


Instrument AVH400
Group HJS
Chemist Suer
COSY.crl DMSO {C:\NMR} hjsgrp 1

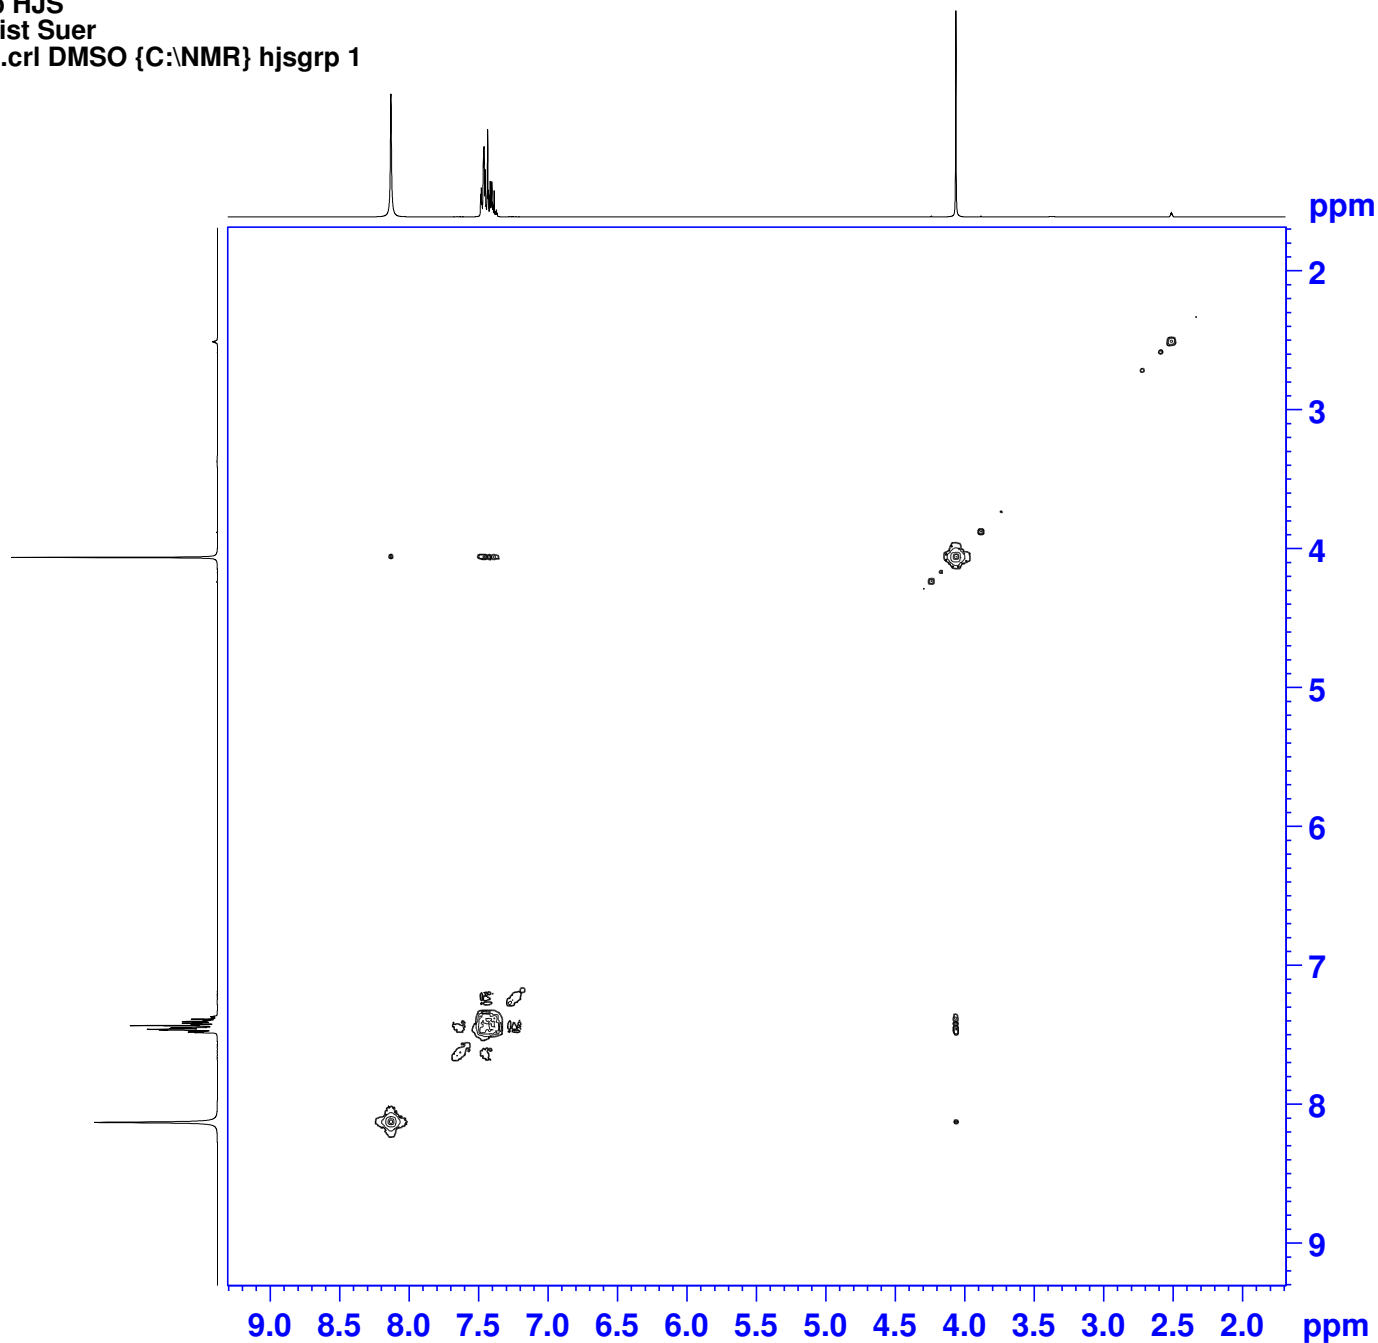

Current Data Parameters
NAME Jul25-2022-1-BzaI
EXPNO 4
PROCNO 1

F2 - Acquisition Parameters
Date_ 20220725
Time 21.07 h
INSTRUM avh400
PROBHD Z116098_0219 (
PULPROG cosygpppqf
TD 2048
SOLVENT DMSO
NS 1
DS 8
SWH 3048.781 Hz
FIDRES 2.977325 Hz
AQ 0.3358720 sec
RG 30.75
DW 164.000 usec
DE 6.50 usec
TE 296.0 K
D0 0.00000300 sec
D1 1.85582101 sec
D11 0.03000000 sec
D12 0.00002000 sec
D13 0.00000400 sec
D16 0.00020000 sec
IN0 0.00032800 sec
TDav 1
SF01 400.1321993 MHz
NUC1 1H
P0 10.00 usec
P1 10.00 usec
P17 2500.00 usec
PLW1 16.00000000 W
PLW10 1.77779996 W
GPNAM[1] SMSQ10.100
GPZ1 10.00 %
P16 1000.00 usec

F1 - Acquisition parameters
TD 128
SF01 400.1322 MHz
FIDRES 47.637196 Hz
SW 7.619 ppm
FnMODE QF

F2 - Processing parameters
SI 1024
SF 400.1300000 MHz
WDW QSINE
SSB 0
LB 0 Hz
GB 0
PC 1.40

F1 - Processing parameters
SI 1024
MC2 QF
SF 400.1300000 MHz
WDW QSINE
SSB 0
LB 0 Hz
GB 0