
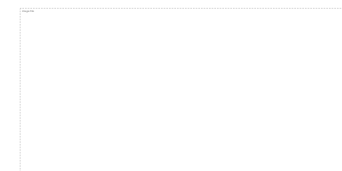


Instrument AVH400
Group HJS
Chemist Suer
h1acqQ.crl DMSO {C:\NMR} hjsgrp 4

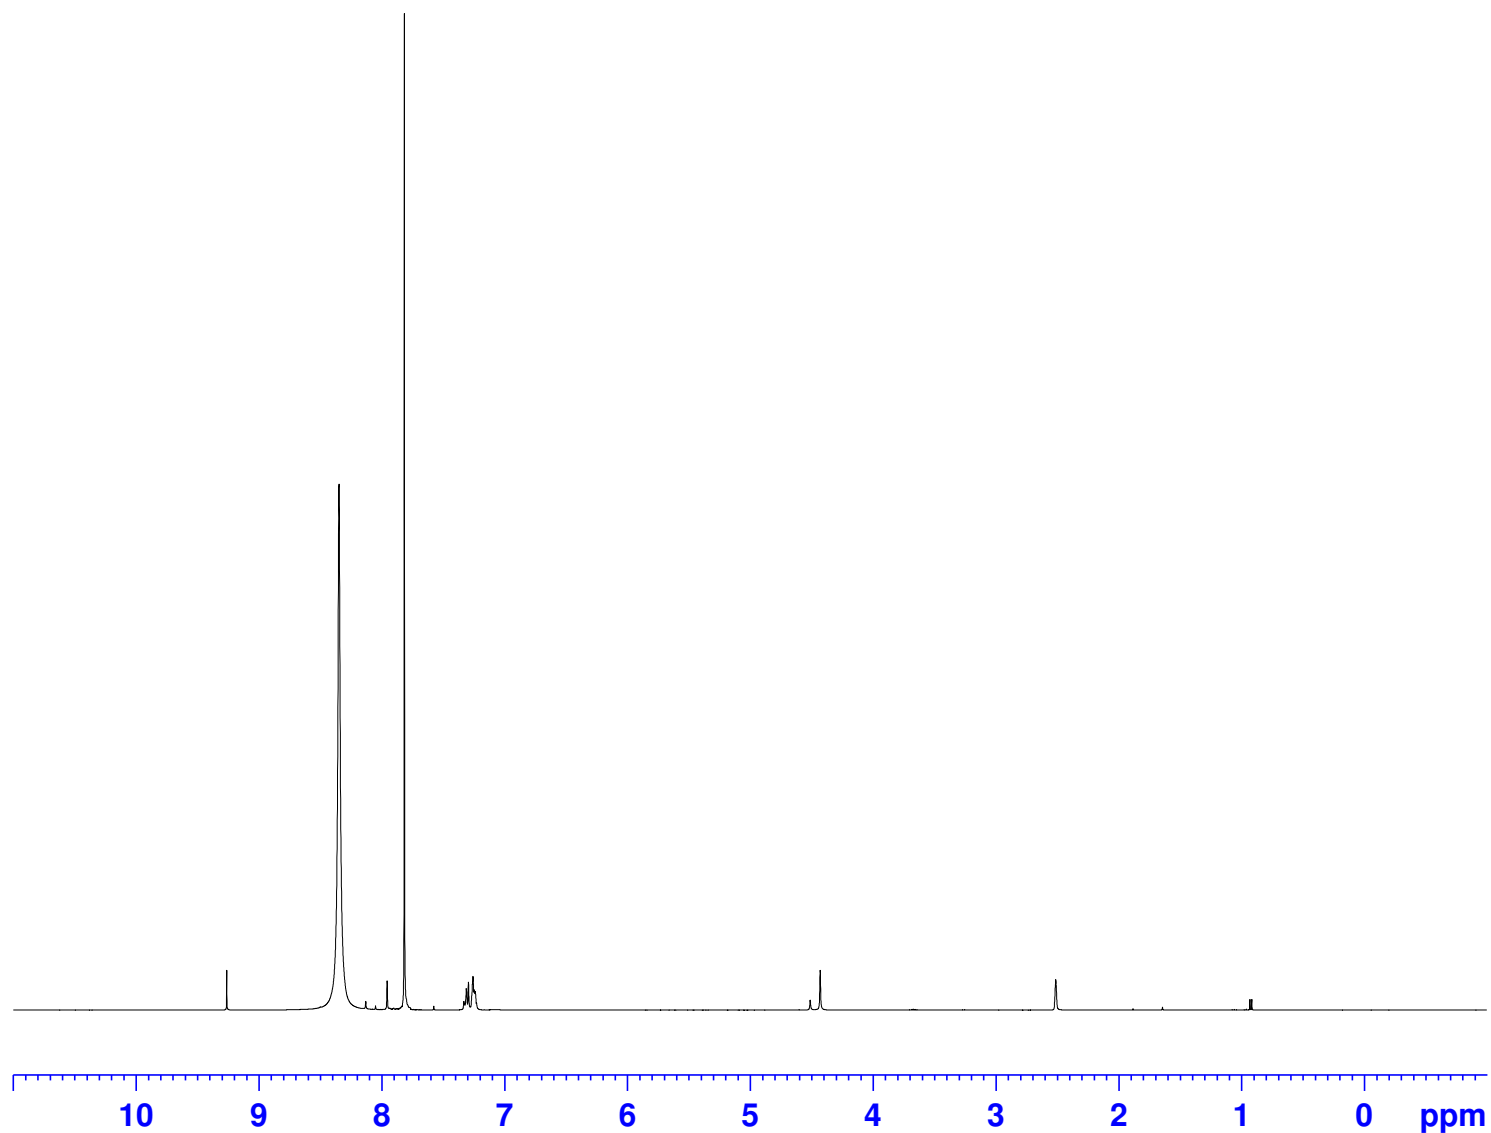

Current Data Parameters
NAME Jul25-2022-4-Cs25Br20 5 percent Bza_aged
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20220725
Time_ 19.54 h
INSTRUM avh400
PROBHD Z116098_0219 (
FULPROG zg
TD 65536
SOLVENT DMSO
NS 4
DS 0
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 15.33
DW 62.400 usec
DE 6.50 usec
TE 296.5 K
D1 25.00000000 sec
TDO 1
SFO1 400.1324008 MHz
NUC1 1H
P1 10.00 usec
PLW1 16.00000000 W

F2 - Processing parameters
SI 32768
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00