


Instrument AVH400  
Group HJS  
Chemist Suer  
c13acq\_256.crl DMSO {C:\NMR} hjsgrp 24

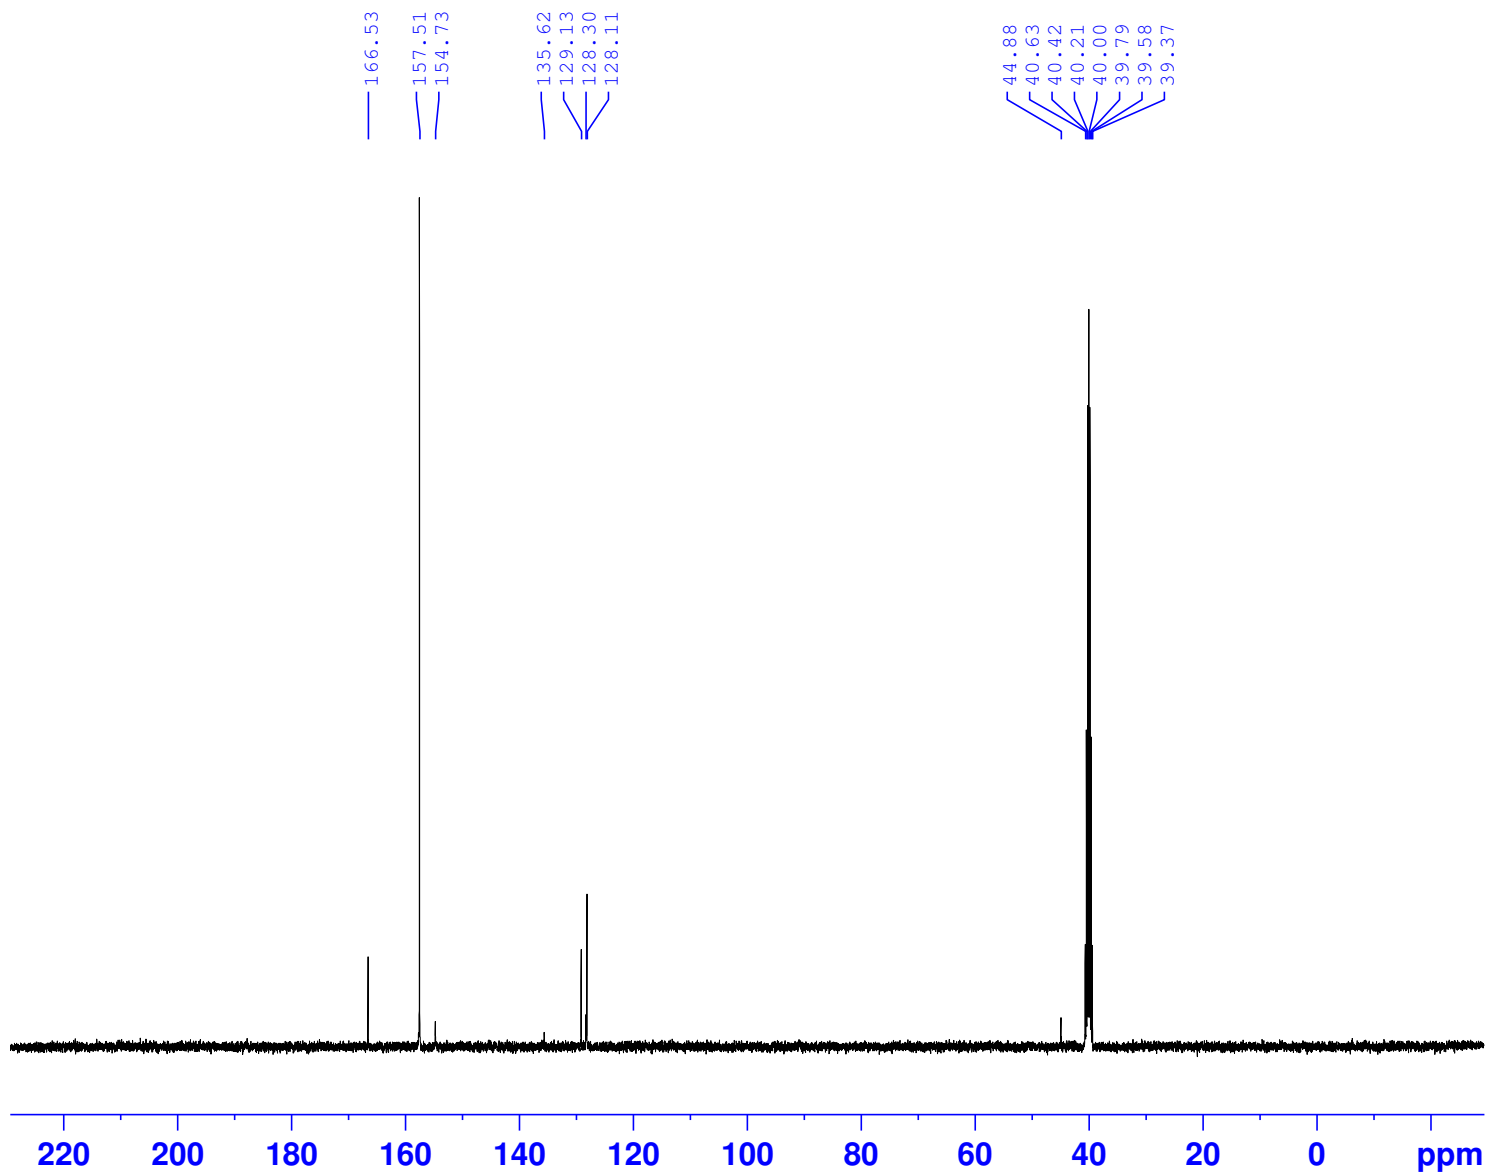

Current Data Parameters  
NAME May19-2022-24-FAI\_5 percent Bza  
EXPNO 1  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20220521  
Time 2.37 h  
INSTRUM avh400  
PROBHD z108618\_0873 (  
PULPROG zgpg30  
TD 32768  
SOLVENT DMSO  
NS 256  
DS 4  
SWH 26041.666 Hz  
FIDRES 1.589457 Hz  
AQ 0.6291456 sec  
RG 197.18  
DW 19.200 usec  
DE 6.50 usec  
TE 299.1 K  
D1 1.00000000 sec  
D11 0.03000000 sec  
TD0 1  
SFO1 100.6228298 MHz  
NUC1 13C  
P0 3.33 usec  
P1 10.00 usec  
PLW1 47.86100006 W  
SFO2 400.1316005 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 14.36999989 W  
PLW12 0.34772000 W  
PLW13 0.17490000 W

F2 - Processing parameters  
SI 32768  
SF 100.6127685 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40