
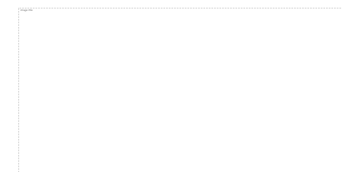


Instrument AVH400
Group HJS
Chemist Suer
COSY.crl DMSO {C:\NMR} hjsgrp 24

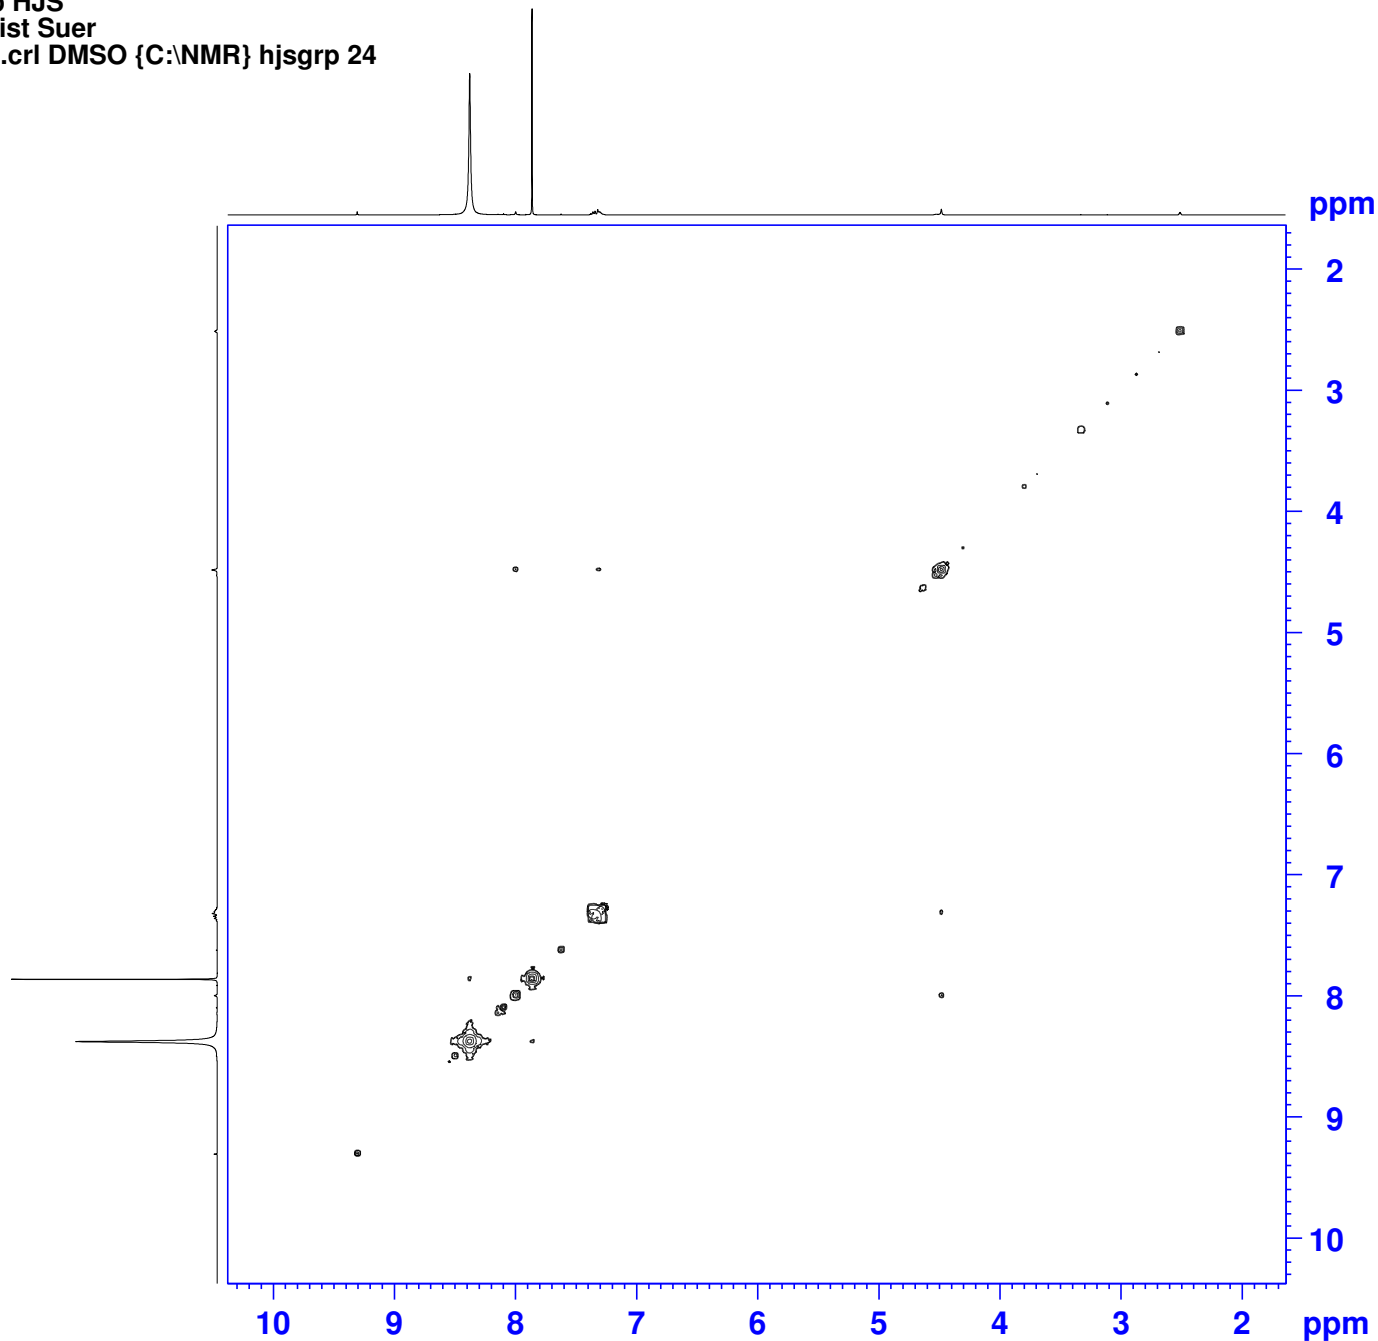

Current Data Parameters
NAME May19-2022-24-FAI_5 percent Bza
EXPNO 3
PROCNO 1

F2 - Acquisition Parameters
Date_ 20220521
Time 2.39 h
INSTRUM avh400
PROBHD Z108618_0873 (
PULPROG cosygpppgf
TD 2048
SOLVENT DMSO
NS 1
DS 8
SWH 3496.503 Hz
FIDRES 3.414554 Hz
AQ 0.2928640 sec
RG 27.09
DW 143.000 usec
DE 6.50 usec
TE 298.5 K
D0 0.00000300 sec
D1 1.89882898 sec
D11 0.03000000 sec
D12 0.00002000 sec
D13 0.00000400 sec
D16 0.00020000 sec
IN0 0.00028600 sec
TDav 1
SFO1 400.1324037 MHz
NUC1 1H
P0 14.00 usec
P1 14.00 usec
P17 2500.00 usec
PLW1 14.36999989 W
PLW10 3.12949991 W
GPNAM[1] SMSQ10.100
GPZ1 10.00 %
P16 1000.00 usec

F1 - Acquisition parameters
TD 128
SFO1 400.1324 MHz
FIDRES 54.632866 Hz
SW 8.738 ppm
FnMODE QF

F2 - Processing parameters
SI 1024
SF 400.1300000 MHz
WDW QSINE
SSB 0
LB 0 Hz
GB 0
PC 1.40

F1 - Processing parameters
SI 1024
MC2 QF
SF 400.1300000 MHz
WDW QSINE
SSB 0
LB 0 Hz
GB 0