
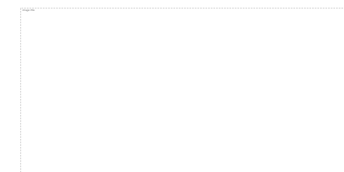


Instrument AVH400  
Group HJS  
Chemist Suer  
COSY.crl DMSO {C:\NMR} hjsgrp 28

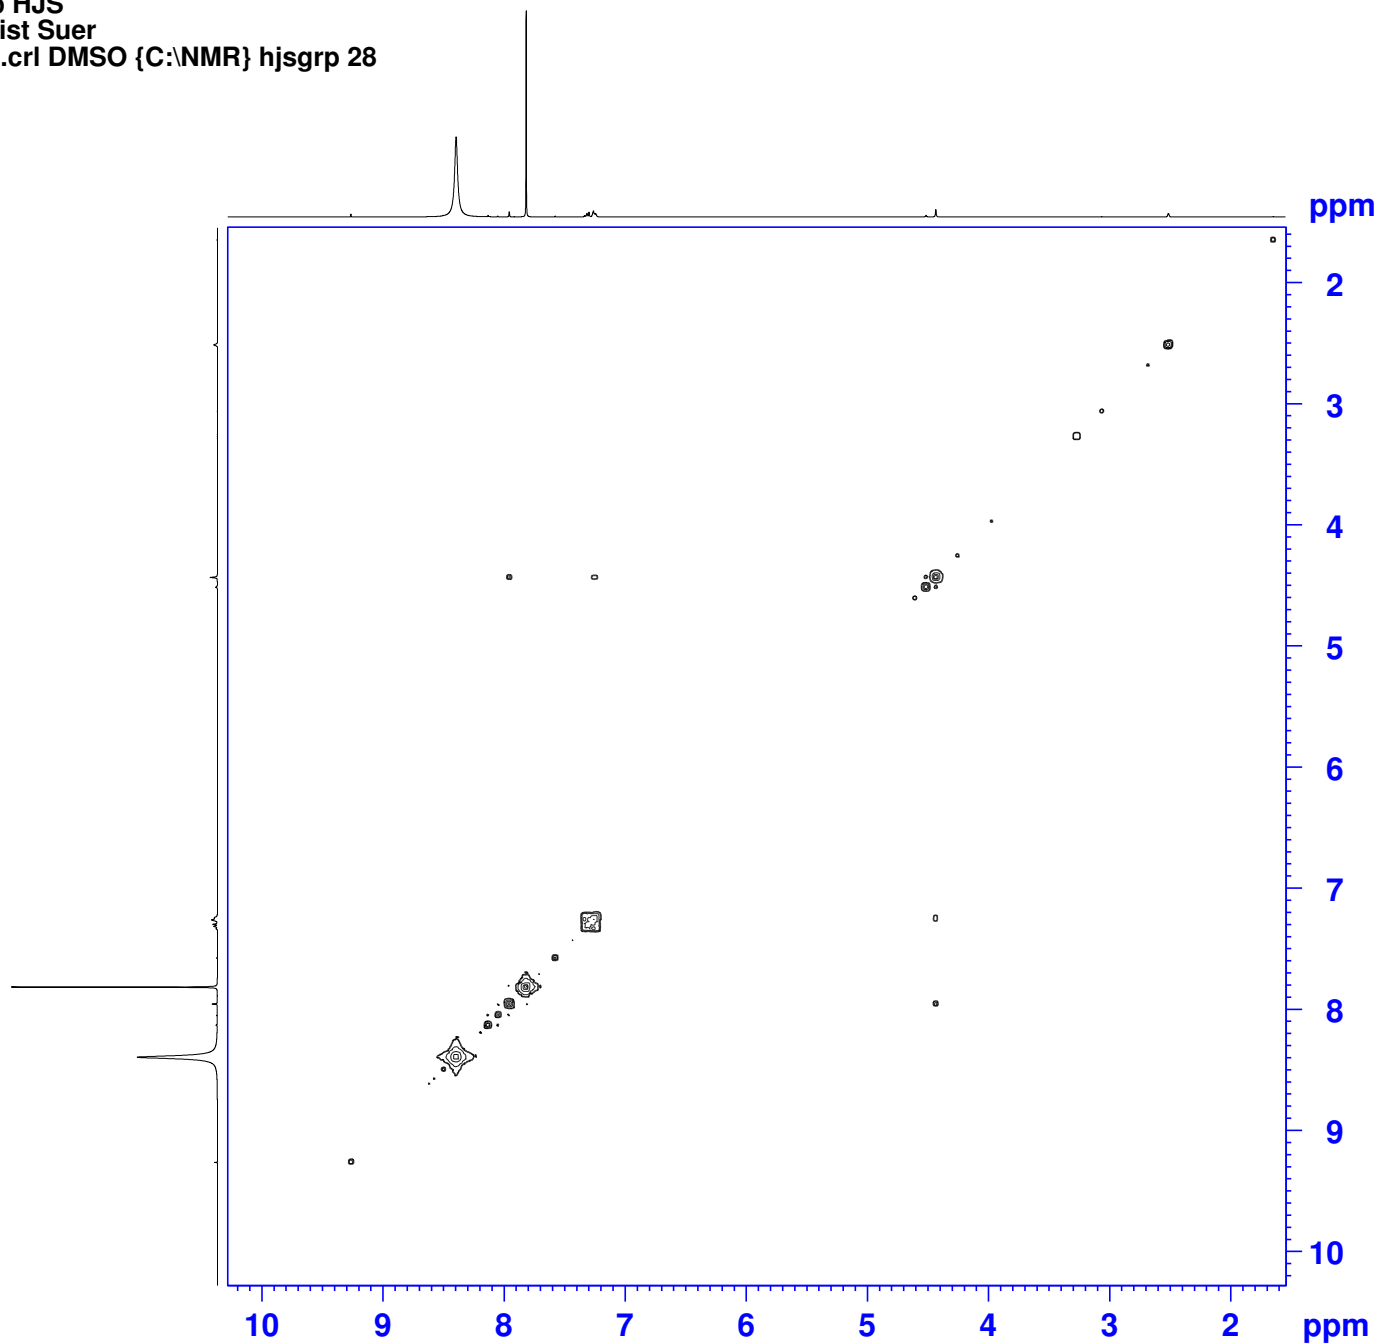

Current Data Parameters  
NAME May19-2022-28-Cs25Br20\_5 percent Bza  
EXPNO 3  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20220521  
Time 3.02 h  
INSTRUM avh400  
PROBHD Z108618\_0873 (  
PULPROG cosygpppqf  
TD 2048  
SOLVENT DMSO  
NS 1  
DS 8  
SWH 3496.503 Hz  
FIDRES 3.414554 Hz  
AQ 0.2928640 sec  
RG 27.09  
DW 143.000 usec  
DE 6.50 usec  
TE 298.5 K  
D0 0.00000300 sec  
D1 1.89882898 sec  
D11 0.03000000 sec  
D12 0.00002000 sec  
D13 0.00000400 sec  
D16 0.00020000 sec  
IN0 0.00028600 sec  
TDav 1  
SFO1 400.1323659 MHz  
NUC1 1H  
P0 14.00 usec  
P1 14.00 usec  
P17 2500.00 usec  
PLW1 14.36999989 W  
PLW10 3.12949991 W  
GPNAM[1] SMSQ10.100  
GPZ1 10.00 %  
P16 1000.00 usec

F1 - Acquisition parameters  
TD 128  
SFO1 400.1324 MHz  
FIDRES 54.632866 Hz  
SW 8.738 ppm  
FnMODE QF

F2 - Processing parameters  
SI 1024  
SF 400.1300000 MHz  
WDW QSINE  
SSB 0  
LB 0 Hz  
GB 0  
PC 1.40

F1 - Processing parameters  
SI 1024  
MC2 QF  
SF 400.1300000 MHz  
WDW QSINE  
SSB 0  
LB 0 Hz  
GB 0