
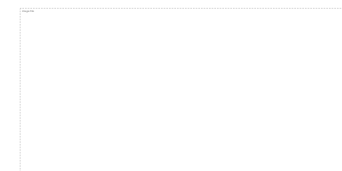


Instrument AVH400  
Group HJS  
Chemist Suer  
h1acq.crl DMSO {C:\NMR} hjsgrp 6

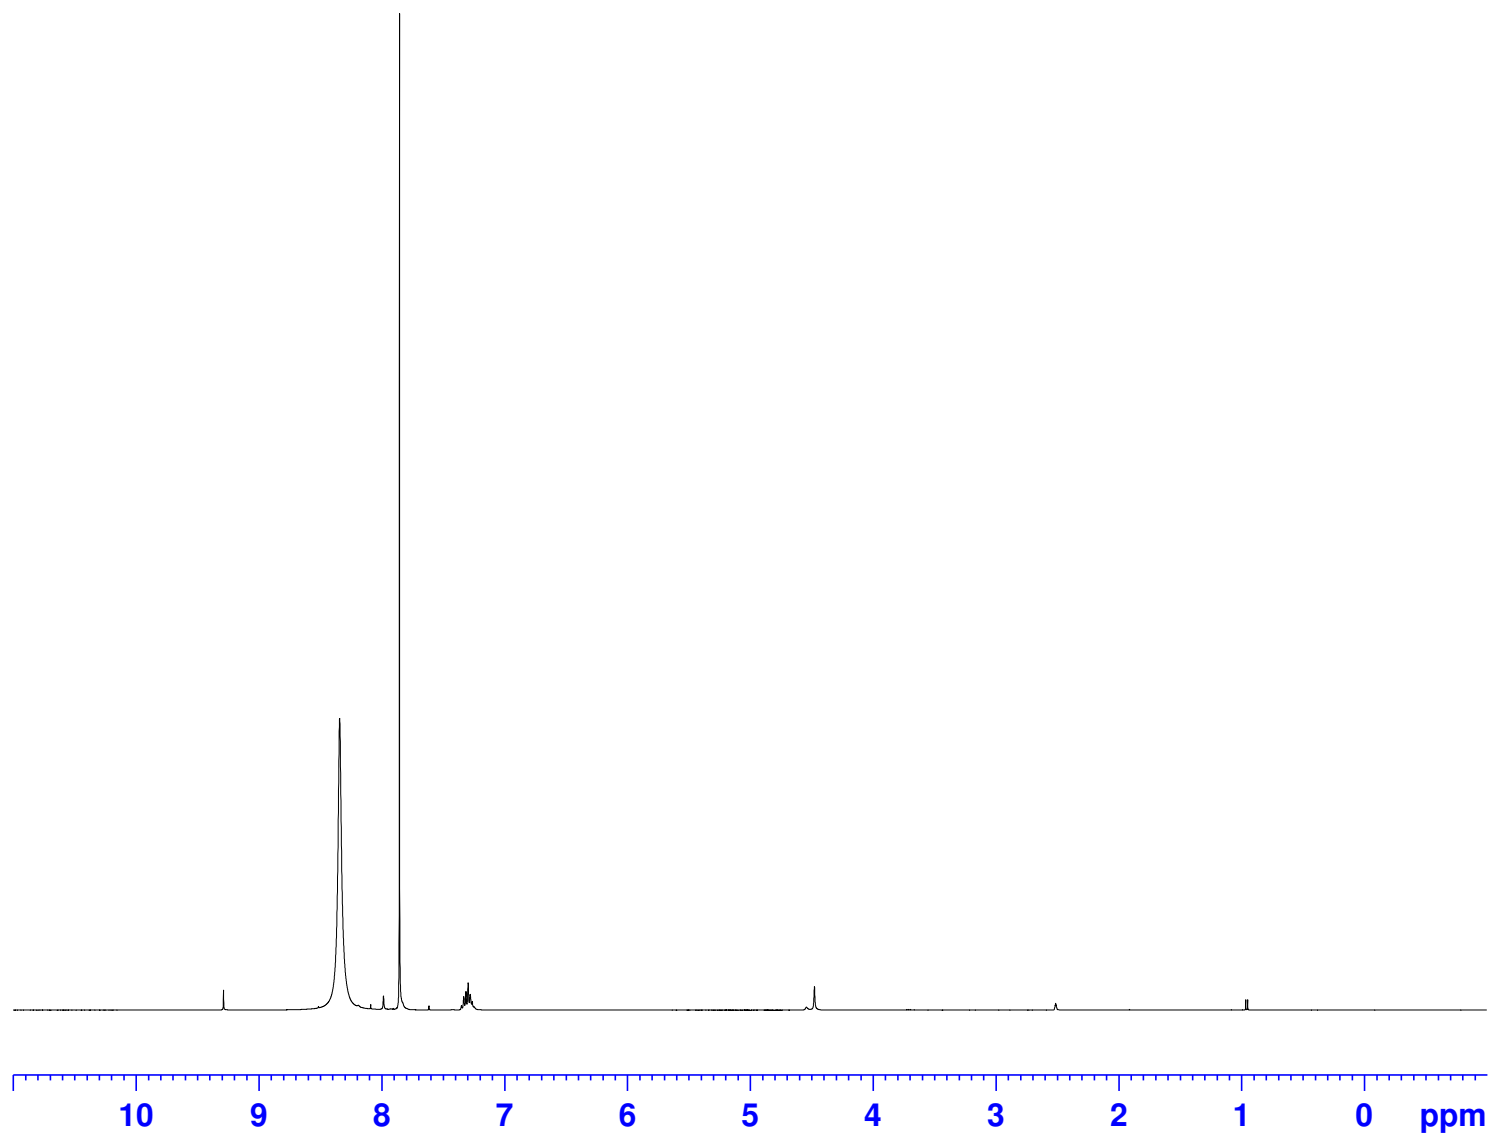

Current Data Parameters  
NAME May19-2022-6-FAI\_5 percent Bza\_aged  
EXPNO 2  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20220521  
Time 4.01 h  
INSTRUM avh400  
PROBHD Z108618\_0873 (  
PULPROG zg60  
TD 65536  
SOLVENT DMSO  
NS 16  
DS 2  
SWH 8012.820 Hz  
FIDRES 0.244532 Hz  
AQ 4.0894465 sec  
RG 19.72  
DW 62.400 usec  
DE 6.50 usec  
TE 298.4 K  
D1 1.00000000 sec  
TD0 1  
SFO1 400.1324008 MHz  
NUC1 1H  
P1 14.00 usec  
PLW1 14.36999989 W

F2 - Processing parameters  
SI 32768  
SF 400.1300000 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00