

Increasing sensitivity and versatility in NMR supersequences with new HSQC-based modules



Jonathan R.J. Yong^a, Alexandar L. Hansen^b, Ēriks Kupče^c, Tim D.W. Claridge^{a,*}

^a Chemistry Research Laboratory, Department of Chemistry, University of Oxford, Mansfield Road, Oxford OX1 3TA, UK

^b Campus Chemical Instrument Center, The Ohio State University, 460 W. 12th Avenue, Columbus, OH 43210, USA

^c Bruker UK Ltd., Banner Lane, Coventry CV4 9GH, UK

ARTICLE INFO

Article history:

Received 31 March 2021

Revised 15 June 2021

Accepted 16 June 2021

Available online 19 June 2021

Keywords:

NMR spectroscopy

NOAH supersequences

Analytical methods

Sensitivity-enhanced HSQC

HSQC-TOCSY

ABSTRACT

The sensitivity-enhanced HSQC, as well as HSQC-TOCSY, experiments have been modified for incorporation into NOAH (NMR by Ordered Acquisition using ¹H detection) supersequences, adding diversity for ¹³C and ¹⁵N modules. Importantly, these heteronuclear modules have been specifically tailored to preserve the magnetisation required for subsequent acquisition of other heteronuclear or homonuclear modules in a supersequence. In addition, we present protocols for optimally combining HSQC and HSQC-TOCSY elements within the same supersequences, yielding high-quality 2D spectra suitable for structure characterisation but with greatly reduced experiment durations. We further demonstrate that these time savings can translate to increased detection sensitivity per unit time.

© 2021 The Authors. Published by Elsevier Inc. This is an open access article under the CC BY license (<http://creativecommons.org/licenses/by/4.0/>).

1. Introduction

In recent years, there has been significant interest in the acceleration of multidimensional NMR data acquisition [1–43]. In particular, some of the more readily implemented methods involve multiple-FID experiments which use either single or multiple receivers. Of these, one of the most versatile approaches is to utilise different “pools” of magnetisation available within a sample for the sequential collection of different spectra without an intervening recovery delay, as exemplified by the NOAH (NMR by Ordered Acquisition using ¹H detection) technique [43–48]. Virtually all of the most common 2D experiments used in small molecule characterisation, such as HSQC, HMBC, COSY, TOCSY, NOESY, and ROESY, can be combined in a modular fashion to form *supersequences* which collectively use only one recovery delay (*d*₁) (Fig. 1a). As the recovery delay accounts for the large majority of experiment time in 2D NMR, the NOAH approach can provide time savings of up to ~4× compared to the conventional individual acquisition of each spectrum, where each constituent experiment would require its own recovery delay.

One-bond heteronuclear correlation experiments, namely HSQC and HMQC, play a central role in the structural elucidation of small organic molecules and biomolecules [49,50]. These experiments

are also a core component of many NOAH experiments, since the magnetisation they use (protons directly coupled to isotopically dilute X nuclei, i.e. ¹³C or ¹⁵N) can be efficiently differentiated from the “bulk” magnetisation of protons that are not directly attached to these NMR-active nuclei [51–56]. Following the notation of Orts [57], we refer to these two magnetisation components (proton coupled to X and proton not coupled to X) as ¹H^X and ¹H^{̄X} respectively. At the same time, due to the low natural abundance of these heteronuclei, these spectra are typically less sensitive than the homonuclear spectra that are placed towards the end of the supersequence. Consequently, for dilute samples, the minimum experimental time is generally dictated by these heteronuclear experiments, meaning any improvements in experiment sensitivity can be directly translated into greater time savings.

In the 1990s, Cavanagh, Rance, and Kay introduced the sensitivity-enhanced HSQC (seHSQC) experiment [58,59], which improves on the sensitivity of an ordinary echo-antiecho HSQC by up to a factor of 2 in the most ideal case. This is accomplished through the so-called preservation of equivalent pathways (PEP) scheme, which converts two magnetisation components that are cosine- and sine-modulated in *t*₁ into observable magnetisation prior to detection [60,61]. Here, we show how the original seHSQC sequence can be modified such that it can be used as a NOAH module, thus bringing about even further gains in sensitivity per unit time. We add further diversification by incorporating a HSQC-TOCSY module, derived from the ASAP-HSQC-TOCSY [10], that is

* Corresponding author.

E-mail address: tim.claridge@chem.ox.ac.uk (T.D.W. Claridge).

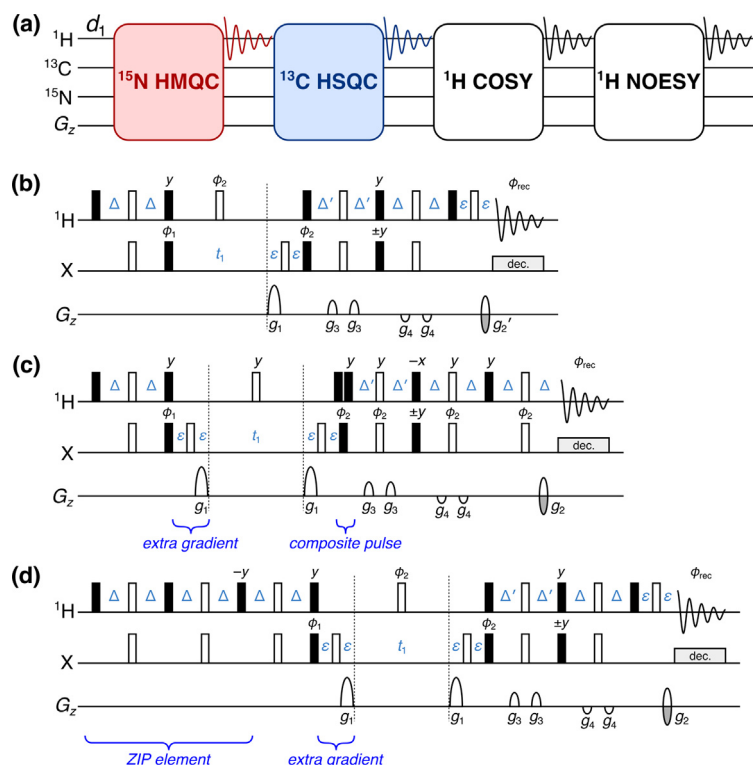


Fig. 1. (a) Overview of a typical NOAH supersequence (MSCN, using the single-letter abbreviations previously defined [44]). The ${}^1\text{H}$ - ${}^{15}\text{N}$ HMQC and ${}^1\text{H}$ - ${}^{13}\text{C}$ HSQC modules are coloured; these may be replaced with the new seHSQC module proposed in this work. (b) Cavanagh-Rance-Kay (CRK) seHSQC [58,59]. (c) Version 1 of the NOAH seHSQC module, abbreviated as “S₁⁺”. (d) Version 2 of the NOAH seHSQC module (“ZIP-seHSQC”), abbreviated as “S₂⁺”. Filled and unfilled bars represent 90° and 180° pulses respectively; all 180° pulses on ${}^{13}\text{C}$ are adiabatic (frequency-swept) pulses. All pulses are applied along +x unless otherwise noted. Phase cycling is performed with $\phi_1 = (x, -x)$, $\phi_2 = (x, x, -x, -x)$, and $\phi_{\text{rec}} = (x, -x, -x, x)$. The delays are chosen as follows: $\Delta = 1/(4 \cdot {}^1J_{\text{XH}})$, $\Delta' = 1/(8 \cdot {}^1J_{\text{CH}})$ or $1/(4 \cdot {}^1J_{\text{NH}})$, and ε is the minimum time needed for a gradient pulse and subsequent recovery. All gradient pulses are 1 ms long, except for g_1 and g_2 in ${}^{15}\text{N}$ experiments which are 2.5 ms long. Gradient amplitudes, as percentages of maximum gradient strength (53 G/cm), are as follows: $g_1 = 80\%$; $g_2 = \pm 40.2\%$ (${}^{13}\text{C}$) or $\pm 16.2\%$ (${}^{15}\text{N}$); $g_2' = g_2/2$; $g_3 = 11\%$; $g_4 = -5\%$. The signs of g_2 and g_2' , as well as the phase of the 90° X pulse marked $\pm y$, are alternated within each t_1 increment to provide echo-antiecho selection. Refer to Figure S1 for product operator analysis.

also compatible with the NOAH strategy. Both of these modules can be inserted either independently or together into NOAH supersequences, allowing large amounts of chemical information to be acquired in short times.

2. Results and discussion

2.1. ${}^1\text{H}$ - ${}^{13}\text{C}$ sensitivity-enhanced HSQC

A typical example of a NOAH supersequence is the NOAH-4 MSCN experiment (Fig. 1a), which yields ${}^{15}\text{N}$ HMQC, ${}^{13}\text{C}$ HSQC, COSY, and NOESY spectra in one single experiment [44]. The implementation of this supersequence relies on the fact that the output of any one module contains all the necessary magnetisation components required for downstream modules. For example, both the standard NOAH HMQC (Figure S1a) [3,44] and HSQC (Figure S1b) [8,44] modules return the bulk ${}^1\text{H}^x$ magnetisation back to its equilibrium position (+z). In the MSCN sequence, this bulk magnetisation can therefore be used as the input to the COSY and NOESY homonuclear modules which follow. However, the original Cavanagh-Rance-Kay (CRK) seHSQC (Fig. 1b) does not obey this principle: it causes bulk magnetisation to be dephased by coherence transfer pathway (CTP) gradients. Consequently, downstream modules can only utilise any bulk ${}^1\text{H}^x$ magnetisation that has relaxed during the HSQC FID acquisition, leading to drastic losses in signal intensity. This is illustrated using a NOAH-2 S⁺C⁺ (seHSQC + CLIP-COSY [62]) supersequence (Fig. 2a): the CLIP-COSY is used in this work as a convenient module for which peak

intensities can be easily quantified, but the conclusions drawn here are fully applicable to any other homonuclear module that is used in its place. While the CRK seHSQC implementation (Fig. 2b) affords significant sensitivity gains (primarily for CH peaks, as predicted by theory [63,64]), the COSY module which follows suffers from an almost complete (~90%) loss of intensity. While one could argue that this is still tolerable for the COSY module, which is the most sensitive of all NOAH modules, these losses are not permissible for inherently less sensitive homonuclear modules such as NOESY and ROESY.

In this work, we compare two possible solutions to this, which form the basis of the NOAH seHSQC modules. In both cases, we require a pulse sequence element which performs a selective 90° rotation on ${}^1\text{H}^x$ magnetisation and leaves ${}^1\text{H}^x$ magnetisation untouched. The first version of the NOAH seHSQC (Fig. 1c, “S₁⁺”) uses a composite ${}^1\text{H}$ pulse immediately following t_1 to accomplish this aim, as both magnetisation components have already diverged by this point. On the other hand, the second (Fig. 1d, “S₂⁺” or “ZIP-seHSQC”) actively differentiates the two components at the start of the sequence by prepending a double heteronuclear spin echo, a strategy recently reported by Hansen et al. [66] This zz isotope-selective (ZIP) pulse element is based on the observation that the bulk ${}^1\text{H}^x$ magnetisation in the seHSQC will be returned to +z if the phase of the initial ${}^1\text{H}$ 90° pulse in the CRK seHSQC is changed by 90° to +y. To generate the required HSQC signal, however, a ${}^1\text{H}$ 90° pulse must still be applied to ${}^1\text{H}^x$ magnetisation. Overall, what is required is therefore a pulse sequence element which simultaneously acts as a 90°_x (or 90°_{-x}) pulse on protons coupled to spin-X,

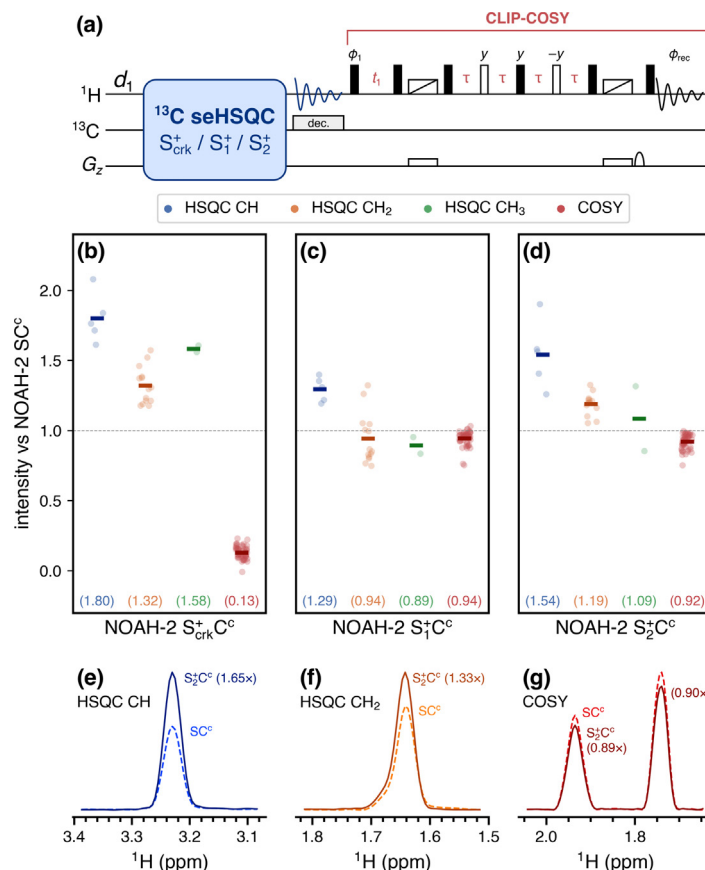


Fig. 2. Sensitivity comparisons for NOAH-2 $S^+ \text{C}^{\text{C}}$ (seHSQC + CLIP-COSY) supersequences, using the CRK and NOAH seHSQC implementations. The delay Δ' was set to $1/(8 \cdot ^1J_{\text{CH}})$. All intensities are normalised against the NOAH-2 SC^{C} (HSQC + CLIP-COSY) supersequence, without HSQC sensitivity enhancement. HSQC intensities are further grouped by multiplicity. Circles represent the relative intensities of individual peaks; solid bars, as well as the numbers in parentheses, indicate averages over all peaks of a given type. (a) Pulse sequence of the NOAH-2 $S^+ \text{C}^{\text{C}}$ (seHSQC + CLIP-COSY) experiment; any of the variants shown in Fig. 1 (CRK, version 1, or version 2/“ZIP”) can be used as the seHSQC module. The CLIP-COSY [62] is performed with $\phi_1 = \phi_{\text{rec}} = (x, -x)$ and States quadrature detection in the indirect dimension; the perfect echo mixing delay τ is set to 8.33 ms. The unfilled rectangles with diagonal lines, applied simultaneously with z-gradients, represent frequency-swept pulses used for suppression of zero-quantum coherence [65]. (b) Using the original CRK seHSQC (Fig. 1b), which leads to severely reduced COSY intensities. (c) Using the S_1^+ module (Fig. 1c). (d) Using the S_2^+ module (Fig. 1d). (e)–(f) Slices of the NOAH HSQC (dashed line) and NOAH ZIP-seHSQC (S_1^+ or S_2^+) spectra (solid line) through $f_1 = 78.9$ ppm (a CH peak, (e)) and $f_1 = 28.5$ ppm (a CH₂ peak, (f)). (g) Slices of the CLIP-COSY module from the NOAH-2 SC^{C} (dashed line) and $S_2^+ \text{C}^{\text{C}}$ (solid line) supersequences, through $f_1 = 1.36$ ppm. Spectra were obtained on a 700 MHz Bruker AV III equipped with a TCI H/C/N cryoprobe; the sample used was 40 mM andrographolide in DMSO- d_6 .

and as a 90_y pulse on uncoupled protons. The resulting ZIP element is similar to the zz-filter, which has previously been used in the NOAH zz-HMBC module to retain the magnetisation of directly coupled protons for a subsequent HSQC module [45,47]. However, the ZIP element has different pulse phases to this and consequently leads to a different overall outcome, i.e. 90_{-x} on $^1\text{H}^{\text{X}}$ and 90_y on $^1\text{H}^{\text{X}}$.

In addition to the aforementioned modifications, both NOAH seHSQC modules also contain a CTP gradient prior to the t_1 period (highlighted in Figs. 1c and d). In the S_1^+ module, the $^1\text{H}^{\text{X}}$ magnetisation is in the xy-plane during t_1 (see Figure S1 for product operator analysis), and would simply be dephased if this gradient were not present, making its presence mandatory. Alternatively, the S_2^+ module places the $^1\text{H}^{\text{X}}$ magnetisation on $\pm z$ in t_1 . This gradient is therefore not used for rephasing, but instead serves to suppress artefacts in downstream modules, which would otherwise arise from bulk magnetisation that (due to pulse imperfections) is not longitudinal and can therefore evolve during either half of the HSQC t_1 period (Figures S2 to S4). This magnetisation then evolves again in the t_1 period of a later homonuclear module (e.g. COSY), resulting in each COSY peak with indirect-dimension frequency $f_1 = \Omega_{\text{H}}$ being accompanied by a pair of “wing” artefacts at $f_1 = \Omega_{\text{H}} \pm (\Omega_{\text{H}} \cdot \text{SW}_{\text{COSY}})/(2 \cdot \text{SW}_{\text{HSQC}})$, where Ω_{H} and SW refer to the proton offset and indirect-dimension spectral width respec-

tively (both in Hz). Importantly, the artefacts arising from diagonal peaks can have intensities that are comparable to genuine cross-peaks (Figure S2), which highlights the importance of suppressing these artefacts. Apart from the “wing” artefacts in downstream modules, we also briefly note here that the presence of two CTP gradients inside the seHSQC t_1 period allows the final CTP gradient (g_2) to have twice its usual amplitude, thereby providing additional artefact suppression in the seHSQC itself. This is particularly important in the ^{15}N seHSQC, as will be explained below.

These pulse sequence modifications result in an unavoidable decrease in efficiency, as compared to the original CRK seHSQC implementation (Figs. 2b to d). For example, with the present sample, when the delay Δ' is set to $1/(8 \cdot ^1J_{\text{CH}})$ as was done here [63], the S_1^+ and S_2^+ modules yield on average a $1.29\times$ and $1.54\times$ boost for CH peaks, which are smaller than the $1.80\times$ increase seen with the CRK seHSQC (the case where $\Delta' = 1/(4 \cdot ^1J_{\text{CH}})$ is explored in Figures S5 and S6). Turning to CH₂ and CH₃ peaks, the use of the S_1^+ module does not provide any enhancement for either of these, whilst the S_2^+ module yields on average a more modest $1.19\times$ and $1.09\times$ sensitivity increase respectively. Nevertheless, it should be emphasised that the S_2^+ module in particular still provides clear sensitivity gains over the reference “gold-standard” NOAH HSQC module, especially for CH and CH₂ peaks (Figs. 2e and f) which are typically less intense.

The major advantage that the NOAH seHSQC modules enjoy over the CRK seHSQC is readily appreciated when considering the homonuclear module which follows. In contrast to the CRK seHSQC, which destroys the requisite bulk $^1\text{H}^{\text{X}}$ magnetisation and is thus unsuitable for use in NOAH supersequences, both of the new seHSQC modules preserve the majority of it, performing $>90\%$ as well as the original HSQC module (Fig. 2g). Altogether, this means that the HSQC intensities in a NOAH supersequence can be substantially boosted using the new seHSQC modules, without compromising the sensitivity of, or introducing extra artefacts in, any homonuclear modules which succeed it. We note that the BIG-BIRD element reported by Briand and Sørensen [55], which independently excites $^1\text{H}^{\text{X}}$ and $^1\text{H}^{\text{Y}}$ magnetisation with arbitrary flip angles and phases, is also capable of performing the same role as the ZIP element in the S_2^+ module. However, we find that the ZIP provides greater signal-to-noise in both the seHSQC itself as well as downstream modules (Figure S7).

Multiplicity editing [67] can be easily incorporated into both NOAH seHSQC modules (Figure S8) by introducing a J -evolution period in the spin echo immediately following t_1 . As described previously, the S_1^+ module places the bulk magnetisation in the xy -plane during the editing period; the same is true of the unenhanced NOAH HSQC. In these modules, the bulk $^1\text{H}^{\text{X}}$ magnetisation is therefore subject to homonuclear coupling (J_{HH}) evolution, leading to a small decrease in the sensitivity of later homonuclear modules when multiplicity editing is introduced. Since homonuclear experiments typically have a greater inherent sensitivity than the (se)HSQC, this minor loss is rarely a problem, and is far outweighed by the benefits of incorporating multiplicity editing in the HSQC. Nevertheless, the fact that the S_2^+ module does not suffer from such a penalty is a welcome benefit. As a result, when editing is included, the S_2^+ module slightly outperforms both the S and S_1^+ modules by around 10% in terms of preserving bulk magnetisation (Figure S9).

2.2. ^1H - ^{15}N sensitivity-enhanced HSQC

The proposed seHSQC modules can be similarly implemented as ^1H - ^{15}N experiments. Currently, in NOAH supersequences, ^1H - ^{15}N correlations are primarily obtained using the HMQC module ("M") [3,44]; compared to this, the new S_2^+ module can provide greater than $4\times$ enhanced sensitivity (Fig. 3). This arises partly because the PEP sensitivity enhancement scheme can be optimised for NH peaks by setting the reverse INEPT transfer delay Δ' to be equal to $1/(4 \cdot ^1J_{\text{NH}})$. However, there is also a significant improvement due to the fact that peaks in the ^{15}N seHSQC are not split in the indirect dimension by J_{HH} , unlike in the HMQC. Although the S_2^+ module retains a slightly smaller amount of $^1\text{H}^{\text{N}}$ magnetisation ($\sim 70\%$, versus $\sim 80\%$ for the HMQC (Figure S10)), this is a worthwhile trade-off, since it is the ^{15}N module which typically has the lowest intrinsic sensitivity in a supersequence.

Although the S and S_1^+ modules also provide sensitivity gains versus the HMQC, they both come with other drawbacks. As previously discussed, these two modules place bulk $^1\text{H}^{\text{N}}$ magnetisation in the xy -plane during the t_1 period. Consequently, the amount of bulk magnetisation that is retained decreases as t_1 is lengthened, leading to line broadening in the indirect dimensions of all downstream modules (Figure S11). Whilst this is not a problem with the ^{13}C HSQC where typical ^{13}C indirect dimension acquisition times are relatively short, the smaller spectral widths in ^{15}N experiments can mean downstream modules suffer moderate losses in both sensitivity and resolution. The S_2^+ module avoids this issue entirely, making it especially well-suited to obtaining ^{15}N correlations; we henceforth refer to it as the S_N^+ module.

One remaining potential issue in the S_N^+ module arises from the cumulative effects of pulse imperfections, which cause a portion of bulk $^1\text{H}^{\text{N}}$ magnetisation to be transverse just prior to detection of the seHSQC signal. Although this only represents a small fraction of the bulk magnetisation, if left uncontrolled, the resulting artefacts typically have intensities that are comparable to the seHSQC cross-peaks (Figure S12). The key to suppressing these artefacts efficiently lies in the final CTP gradient g_2 (Fig. 1d), which dephases any transverse bulk magnetisation. The S_N^+ module therefore greatly benefits from having two CTP gradients g_1 within the t_1 period, as this means that g_2 will have twice its usual amplitude. For optimal performance, however, one further modification proves beneficial: the CTP gradients g_1 and g_2 should all be lengthened from their typical duration of 1 ms, in order to provide more effective dephasing. In practice, we find that gradient durations of 2 to 2.5 ms provide excellent artefact suppression whilst not causing any appreciable difference in the intensity of the desired cross-peaks (Figure S12). These extended gradients are not required in the ^{13}C seHSQC for two reasons: firstly, the amplitude of g_2 in the ^{13}C seHSQC is larger by a factor of $\gamma_{\text{C}}/\gamma_{\text{N}} \approx 2.5$; and secondly, the greater natural abundance of ^{13}C (1.1% versus 0.36% of ^{15}N) leads to an intrinsically larger signal intensity, which makes any residual artefacts less apparent.

In scenarios where high resolution in the ^{15}N dimension is not required, it is possible to reduce the indirect-dimension (F_1) resolution in order to obtain sensitivity gains. This can be done either by increasing the F_1 spectral width by a factor of k ("SW-scaling"), or by reducing the number of t_1 increments by a factor of k and in its place increasing the number of transients (" k -scaling") [25,26]: both of these cause equivalent reductions of the F_1 acquisition time and thus resolution (Figure S13). When implemented within a supersequence, this scaling is applied exclusively to the ^{15}N module: all other modules are left untouched. In our hands, significant sensitivity gains of up to $\sim 2\times$ can be observed in SW- and k -scaled ^{15}N HMQC spectra, since J_{HH} splitting in the indirect dimension tends not to be resolved (Figure S14). This point is not relevant to the seHSQC, and here, any scaling employed in isolation has only a small effect on peak height, since any peak volume gained from the extra transients is typically offset by the broadening (Figure S15). It is possible to use linear prediction [68–70] to counteract this broadening, thereby improving the signal-to-noise ratio (SNR) of the resulting spectra (Figures S16 and S17). We note, however, that SNR improvements obtained purely via processing methods such as linear prediction should not be conflated with an increase in the true detection sensitivity of the spectrum [71–73].

2.3. HSQC-TOCSY

Thus far, we have described seHSQC modules which utilise all of the $^1\text{H}^{\text{X}}$ magnetisation. However, it is often desirable to draw on $^1\text{H}^{\text{C}}$ magnetisation for multiple different purposes: for example, one can simultaneously collect ^{13}C -decoupled and coupled HSQC spectra [38], HSQC spectra with different spectral widths [39], or a combination of HSQC and HSQC-TOCSY spectra [38]. This has previously been accomplished in a multi-FID acquisition (MFA) scheme by keeping the two CTPs in the CRK seHSQC separate, with the cosine- and sine-modulated CTPs each contributing to one spectrum [38,39]. We chose to adopt a different approach for NOAH supersequences, which exploits the fact that the HSQC module (though not the new seHSQC modules) allows an arbitrary amount of $^1\text{H}^{\text{C}}$ magnetisation to be excited, with the remainder returned to $+z$ [3,7–9]. In order to excite a proportion f of $^1\text{H}^{\text{C}}$ magnetisation ($0 < f \leq 1$), the initial INEPT delay must be shortened by

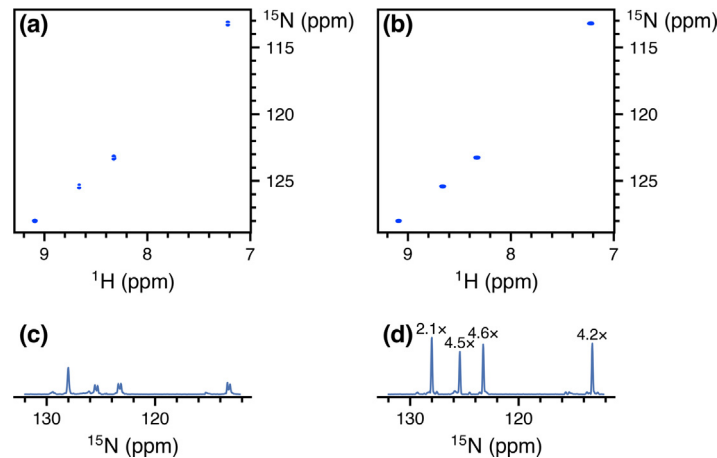


Fig. 3. Comparison of the ^1H - ^{15}N seHSQC module (S_2^+) with the standard NOAH HMQC module (M), taken from NOAH-3 $\text{X}^{\text{S}^+}\text{C}^{\text{C}}$ supersequences (^{15}N experiment + ^{13}C seHSQC + CLIP-COSY). The S_1^+ module is not shown here as it causes line broadening in downstream modules (see text). (a) $\text{X} = \text{M}$, i.e. ^{15}N HMQC module. (b) $\text{X} = S_2^+$, i.e. ^{15}N seHSQC module. (c) Projection of HMQC onto the f_1 axis. Splitting due to J_{HH} is clearly visible for three of the four peaks. (d) Projection of seHSQC onto the f_1 axis. Sensitivity improvements relative to the HMQC spectrum (as measured by peak heights) are indicated above each peak. The largest gains are observed for peaks where the multiplet structure is collapsed; however, even in the absence of that, a $\sim 2\times$ gain is still obtained. Spectra were obtained on a 700 MHz Bruker AV III equipped with a TCI H/C/N cryoprobe; the sample used was 40 mM gramicidin (a cyclic decapeptide; (Val-Orn-Leu-D-Phe-Pro) $_2$) in DMSO- d_6 .

a factor of $\arcsin f$ (Fig. 4a). The remaining $(1 - f)$ of the magnetisation, plus any that relaxes during the HSQC FID, can then be used for a *second* HSQC-based module in the same supersequence. With the present NOAH strategy, for values of f close to 1, the amount of $^1\text{H}^{\text{C}}$ magnetisation regained through relaxation can reach almost 50%. Consequently, by setting $f \approx 0.8$, we can obtain two HSQC spectra with sensitivities that are comparable to the existing MFA approach. Furthermore, the sensitivity of the second HSQC can be boosted by using the new seHSQC modules in its place, in particular the S_2^+ module (Figure S18).

By adding a period of isotropic mixing prior to detection, the NOAH HSQC module may be converted to a HSQC-TOCSY module

(denoted by “ S^{T} ”, Fig. 4b). This is similar to the previously reported ASAP-HSQC-TOCSY [10], the key difference being that in the present NOAH context, unused $^1\text{H}^{\text{C}}$ as well as bulk $^1\text{H}^{\text{C}}$ magnetisation is preserved for use in other modules, instead of later t_1 increments as in the ASAP experiment. Compared to the existing MFA HSQC-TOCSY/HSQC experiment [38], our approach has several characteristics which make it particularly amenable to use in NOAH supersequences. Firstly, the vast majority of $^1\text{H}^{\text{C}}$ magnetisation is preserved, as required for homonuclear module(s) to be appended in a NOAH supersequence (Fig. 4c); in practice, we observe small $^1\text{H}^{\text{C}}$ losses of ca. 10% due to pulse imperfections. In contrast, the MFA sequence, much like the original CRK seHSQC on which it is

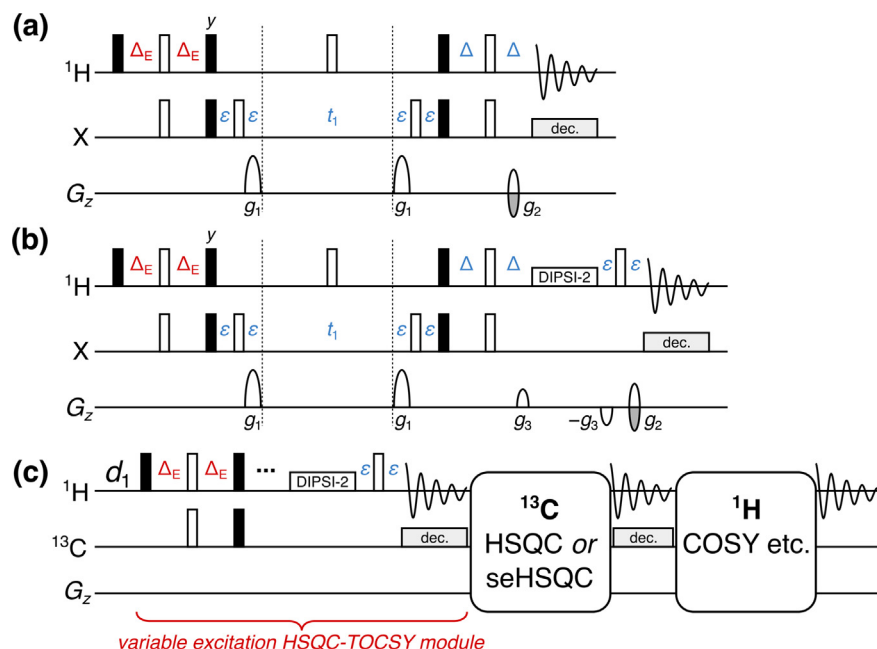


Fig. 4. (a) NOAH HSQC module with modified INEPT delay $\Delta_E = (\arcsin f)/(4 \cdot J_{\text{CH}})$, where f is the fraction of $^1\text{H}^{\text{C}}$ magnetisation excited. (b) NOAH HSQC-TOCSY module (“ S^{T} ”), modified from the ASAP-HSQC-TOCSY [10]. The gradients g_3 are 1 ms long and have an amplitude of 10.1 G/cm. (c) Overview of a NOAH-3 $\text{S}'\text{X}$ or $\text{S}^{\text{T}}\text{X}$ supersequence. The $^1\text{H}^{\text{C}}$ magnetisation is partly used by the initial HSQC-TOCSY module, with a subsequent HSQC or seHSQC using the remaining $^1\text{H}^{\text{C}}$ magnetisation. The bulk $^1\text{H}^{\text{C}}$ magnetisation is retained for one or more homonuclear modules at the end. All other symbols have the same meanings as in Fig. 1.

based, dephases $^1\text{H}^{\text{C}}$ magnetisation and causes a 80–90% sensitivity loss in downstream spectra. Secondly, since each NOAH module is independently executed, the NOAH approach allows multiplicity editing to be selectively enabled for only the HSQC and not the HSQC-TOCSY: in an edited HSQC-TOCSY, sensitivity will be reduced and any accidental overlap may further lead to crosspeaks being lost unexpectedly. Lastly, the sensitivity of both spectra in a NOAH experiment can be optimised through the value of f ; this allows a larger amount of $^1\text{H}^{\text{C}}$ magnetisation to be used for the inherently less sensitive HSQC-TOCSY. In our experience, setting $f = 0.9$ provides a good balance for $\text{S}^{\text{T}}\text{S}^{\text{C}}$ combinations: the sensitivity in the HSQC is boosted not only by relaxation during the HSQC-TOCSY FID, but also by the isotropic mixing in the HSQC-TOCSY module, which effects a degree of $^1\text{H}^{\text{C}} \rightarrow ^1\text{H}^{\text{C}}$ polarisation transfer (Figure S19). Alternatively, the signal intensity of the HSQC-TOCSY can be maximised by replacing it with the seHSQC-TOCSY module, derived from the S_2^+ module [66]. The seHSQC-TOCSY does still retain $^1\text{H}^{\text{C}}$ magnetisation needed for the terminal homonuclear module(s), but has a minor drawback in that it does not allow for variable $^1\text{H}^{\text{C}}$ excitation and therefore cannot preserve a portion of $^1\text{H}^{\text{C}}$ magnetisation for HSQC modules that follow it (Figure S20).

2.4. Examples of new NOAH supersequences

There exist many ways in which the new modules discussed above can be included in practical experiments for structure characterisation. Here, we illustrate this with the NOAH-4 $\text{S}_\text{N}^+\text{S}_2^+\text{S}_2^+\text{C}^{\text{C}}$ (^{15}N seHSQC, ^{13}C HSQC-TOCSY, ^{13}C seHSQC, and CLIP-COSY) supersequence (Fig. 5). While individual collection of the four spectra above required 57 min and 8 s, the NOAH-4 supersequence took only 17 min and 35 s; this is 31% of the original duration, or equivalently a $3.3\times$ speedup. For typical organic molecules, new supersequences such as the NOAH-4 $\text{S}^{\text{T}}\text{S}_2^+\text{CT}$ allow the rapid and complete collection of C–H and H–H correlations (Figure S21). Experiment times can be further reduced through the use of non-

uniform sampling [74–77] (Figure S22), which is compatible with nearly all of the supersequences shown here (the exceptions being when k -scaling is employed in ^{15}N modules, or when COSY modules are recorded without phase-sensitive detection). One can also prepend the NOAH zz-HMBC module (“B”) [45,47]; this uses the semi-adiabatic zz-filter to preserve both $^1\text{H}^{\text{C}}$ and $^1\text{H}^{\text{N}}$ magnetisation, which can then be sampled in the HSQC-based modules presented here (Figure S23).

2.5. Sensitivity per unit time analysis

The benefits of the time savings afforded by NOAH supersequences are manifold. On top of the greatly increased sample throughput that results from faster acquisition, the combination of multiple modules in a single experiment also ensures that all constituent spectra are recorded under the same experimental conditions, such as temperature. This avoids the need for separate chemical shift referencing in each spectrum, and also makes the real-time monitoring and characterisation of reactive intermediates possible, especially when combined with non-uniform sampling. It is also of note that time savings may be directly translated into increases in sensitivity per unit time. The *relative sensitivity per unit time*, ε_t , of a given module is the product of an *amplitude factor* R_s indicating the intrinsic sensitivity of a module with respect to a reference experiment, and the square root of a *time-saving factor* ρ_t , which reflects the decrease in time needed for collection of all spectra [47,48].

We demonstrate this with the NOAH-4 $\text{S}_\text{N}^+\text{S}_2^+\text{S}_2^+\text{CT}$ supersequence (experimental time of 17 min and 28 s), choosing individually acquired versions of the four constituent modules as the reference spectra (total experimental time of 58 min and 42 s), which gives $\rho_t = 3.36$. The amplitude factor R_s starts off at 1 for the first module, with a slight decrease as the supersequence progresses due to imperfections in magnetisation preservation. Nevertheless, ε_t remains well above 1 for all four modules (Fig. 6), which clearly illustrates the attainable gains in sensitivity per unit time in NOAH

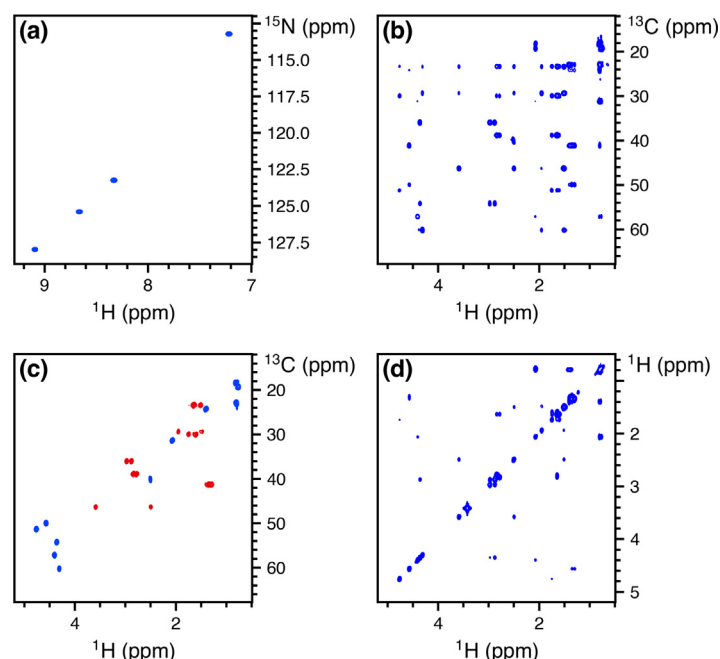


Fig. 5. Spectra obtained from the NOAH-4 $\text{S}_\text{N}^+\text{S}_2^+\text{S}_2^+\text{C}^{\text{C}}$ supersequence. 256 t_1 increments were used, with 2 scans per increment. The total experiment time was 17 min and 35 s. (a) ^{15}N seHSQC. (b) ^{13}C HSQC-TOCSY (30 ms mixing, $f = 0.9$). (c) Multiplicity-edited ^{13}C ZIP-seHSQC. Notice that having the edited seHSQC removes the need for the less desirable HSQC-TOCSY editing. (d) CLIP-COSY. Spectra were obtained on a 700 MHz Bruker AV III equipped with a TCI H/C/N cryoprobe; the sample used was 40 mM gramicidin in $\text{DMSO}-d_6$.

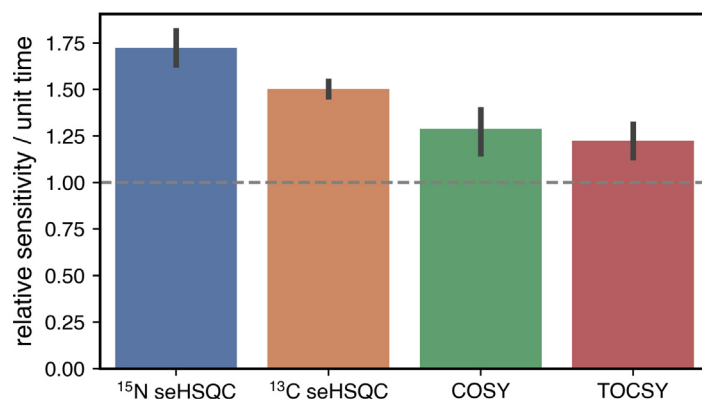


Fig. 6. Relative sensitivities per unit time (ρ_t) for the four modules in the $S_N S_C$ CT supersequence (using a TOCSY mixing time of 35 ms). Error bars indicate 95% confidence intervals. The four NOAH modules, individually acquired, were used as the reference spectra ($\rho_t = 3.36$). Spectra were obtained on a 700 MHz Bruker AV III equipped with a TCI H/C/N cryoprobe; the sample used was 50 mM zolmitriptan in DMSO- d_6 .

sequences where R_S is not significantly compromised: this is especially important for the heteronuclear modules which are naturally less sensitive. Comparisons against “standard” experiments (such as the CRK seHSQC) lead to similar conclusions (Figure S24).

3. Conclusion

The new seHSQC and HSQC-TOCSY implementations add to the preexisting variety of NOAH modules, expanding the number of plausible NOAH supersequences tailored for small molecule characterisation. The controlled manipulation of all proton magnetisation reservoirs present within a sample is required for the success of these modules within nested experiments. We have demonstrated the optimisation of the individual HSQC-based modules and their combinations to further enhance the sensitivity and versatility of NOAH supersequences for efficient data collection.

4. Experimental

All spectra were recorded on a Bruker AV III NMR spectrometer operating at 700 MHz ^1H frequency equipped with a TCI H/C/N cryoprobe. Unless otherwise specified, spectra were recorded with 16 dummy scans, 2 scans per t_1 increment, 256 t_1 increments per module, and a 1.5 s recovery delay. 1024 points were recorded in each FID, leading to an acquisition time of 60.8–73.1 ms depending on the ^1H spectral width (10–12 ppm). Unless otherwise stated, indirect-dimension spectral widths were 180 ppm for ^{13}C modules, and 30 or 80 ppm for ^{15}N modules acquired on gramicidin and zolmitriptan respectively. The delays in the HSQC sequences were optimised for $^1J_{\text{CH}} = 145$ Hz and $^1J_{\text{NH}} = 90$ Hz respectively, and the CLIP-COSY mixing delay (denoted by τ in Fig. 2a) was set to 8.33 ms, corresponding to a nominal J_{HH} value of 30 Hz. DIPSI-2 mixing in the HSQC-TOCSY and TOCSY modules was applied with a B_1 amplitude of 10 kHz.

All NOAH data were processed using the `splitx_au` AU programme, available in the standard Bruker TopSpin software, which separates the individual modules into different datasets; these were then individually processed with `noah_EXPT` AU programmes, which define other processing parameters such as window functions for each module. All datasets were linear predicted up to 512 complex points in f_1 , then zero-filled to 1024 and 2048 complex points in f_1 and f_2 respectively. NUS experiments, such as that in Figure S22, can be set up using a Python script. The pulse sequences used here, all AU processing scripts, as well as the NUS Python script have been made available via the online Bruker User Library ([\[services/bruker-user-library.html\]\(https://www.bruker.com/en/services/bruker-user-library.html\)\), and can also be obtained from Zenodo \(<https://doi.org/10.5281/zenodo.4937946>\). Additionally, the Zenodo deposit also contains all raw NMR data used in this paper.](https://www.bruker.com/en/</p>
</div>
<div data-bbox=)

Declaration of Competing Interest

The authors declare that they have no known competing financial interests or personal relationships that could have appeared to influence the work reported in this paper.

Acknowledgements

We thank Drs. Mohammadali Foroozandeh (University of Oxford) and Peter Howe (Syngenta UK) for helpful discussions. J. R.J.Y. thanks the Clarendon Fund (University of Oxford) and the EPSRC Centre for Doctoral Training in Synthesis for Biology and Medicine (EP/L015838/1) for a studentship, generously supported by AstraZeneca, Diamond Light Source, Defence Science and Technology Laboratory, Evotec, GlaxoSmithKline, Janssen, Novartis, Pfizer, Syngenta, Takeda, UCB, and Vertex.

Appendix A. Supplementary material

Supplementary data associated with this article can be found, in the online version, at <https://doi.org/10.1016/j.jmr.2021.107027>.

References

- [1] P. Schanda, Ě. Kupĉe, B. Brutscher, SOFAST-HMQC experiments for recording two-dimensional heteronuclear correlation spectra of proteins within a few seconds, *J. Biomol. NMR* 33 (2005) 199–211, <https://doi.org/10.1007/s10858-005-4425-x>.
- [2] P. Schanda, H. Van Melckebeke, B. Brutscher, Speeding up three-dimensional protein NMR experiments to a few minutes, *J. Am. Chem. Soc.* 128 (2006) 9042–9043, <https://doi.org/10.1021/ja062025p>.
- [3] Ě. Kupĉe, R. Freeman, Fast multidimensional NMR by polarization sharing, *Magn. Reson. Chem.* 45 (2007) 2–4, <https://doi.org/10.1002/mrc.1931>.
- [4] P. Schanda, Fast-pulsing longitudinal relaxation optimized techniques: Enriching the toolbox of fast biomolecular NMR spectroscopy, *Prog. Nucl. Magn. Reson. Spectrosc.* 55 (2009) 238–265, <https://doi.org/10.1016/j.pnmrs.2009.05.002>.
- [5] J. Furrer, A robust, sensitive, and versatile HMBC experiment for rapid structure elucidation by NMR: IMPACT-HMBC, *Chem. Commun.* 46 (2010) 3396–3398, <https://doi.org/10.1039/C000964D>.
- [6] B. Vitorge, G. Bodenhausen, P. Peluquessy, Speeding up nuclear magnetic resonance spectroscopy by the use of SMALL Recovery Times – SMART NMR, *J. Magn. Reson.* 207 (2010) 149–152, <https://doi.org/10.1016/j.jmr.2010.07.017>.
- [7] D. Schulze-Sünninghausen, J. Becker, B. Luy, Rapid heteronuclear single quantum correlation NMR spectra at natural abundance, *J. Am. Chem. Soc.* 136 (2014) 1242–1245, <https://doi.org/10.1021/ja411588d>.

- [8] D. Schulze-S  nninghausen, J. Becker, M.R.M. Koos, B. Luy, Improvements, extensions, and practical aspects of rapid ASAP-HSQC and ALSOFAST-HSQC pulse sequences for studying small molecules at natural abundance, *J. Magn. Reson.* 281 (2017) 151–161, <https://doi.org/10.1016/j.jmr.2017.05.012>.
- [9] M.R.M. Koos, B. Luy, Polarization recovery during ASAP and SOFAST/ALSOFAST-type experiments, *J. Magn. Reson.* 300 (2019) 61–75, <https://doi.org/10.1016/j.jmr.2018.12.014>.
- [10] J. Becker, M.R.M. Koos, D. Schulze-S  nninghausen, B. Luy, ASAP-HSQC-TOCSY for fast spin system identification and extraction of long-range couplings, *J. Magn. Reson.* 300 (2019) 76–83, <https://doi.org/10.1016/j.jmr.2018.12.021>.
- [11] L. Frydman, T. Scherf, A. Lupulescu, The acquisition of multidimensional NMR spectra within a single scan, *Proc. Natl. Acad. Sci. U.S.A.* 99 (2002) 15858–15862, <https://doi.org/10.1073/pnas.252644399>.
- [12] P. Pelupessy, Adiabatic single scan two-dimensional NMR spectroscopy, *J. Am. Chem. Soc.* 125 (2003) 12345–12350, <https://doi.org/10.1021/ja034958g>.
- [13] L. Frydman, A. Lupulescu, T. Scherf, Principles and features of single-scan two-dimensional NMR spectroscopy, *J. Am. Chem. Soc.* 125 (2003) 9204–9217, <https://doi.org/10.1021/ja030055b>.
- [14] P. Giraudeau, L. Frydman, Ultrafast 2D NMR: An emerging tool in analytical spectroscopy, *Annu. Rev. Anal. Chem.* 7 (2014) 129–161, <https://doi.org/10.1146/annurev-anchem-071213-020208>.
- [15] M. Gal, M. Mishkovsky, L. Frydman, Real-time monitoring of chemical transformations by ultrafast 2D NMR spectroscopy, *J. Am. Chem. Soc.* 128 (2006) 951–956, <https://doi.org/10.1021/ja0564158>.
- [16] P. Giraudeau, Y. Shrot, L. Frydman, Multiple ultrafast, broadband 2D NMR spectra of hyperpolarized natural products, *J. Am. Chem. Soc.* 131 (2009) 13902–13903, <https://doi.org/10.1021/ja905096f>.
- [17] A. Herrera, E. Fern  ndez-Valle, R. Mart  nez-  lvarez, D. Molero, Z.D. Pardo, E. S  ez, M. Gal, Real-time monitoring of organic reactions with two-dimensional ultrafast TOCSY NMR spectroscopy, *Angew. Chem. Int. Ed.* 48 (2009) 6274–6277, <https://doi.org/10.1002/anie.200902387>.
- [18] Z.D. Pardo, G.L. Olsen, M.E. Fern  ndez-Valle, L. Frydman, R. Mart  nez-  lvarez, A. Herrera, Monitoring mechanistic details in the synthesis of pyrimidines via real-time, ultrafast multidimensional NMR spectroscopy, *J. Am. Chem. Soc.* 134 (2012) 2706–2715, <https://doi.org/10.1021/ja20154g>.
- [19] K.J. Donovan, E. Kupĉe, L. Frydman, Multiple parallel 2D NMR acquisitions in a single scan, *Angew. Chem. Int. Ed.* 52 (2013) 4152–4155, <https://doi.org/10.1002/anie.201210070>.
- [20] J.-N. Dumez, Spatial encoding and spatial selection methods in high-resolution NMR spectroscopy, *Prog. Nucl. Magn. Reson. Spectrosc.* 109 (2018) 101–134, <https://doi.org/10.1016/j.pnmrs.2018.08.001>.
- [21] B. Gouilleux, L. Rouger, P. Giraudeau, Ultrafast 2D NMR: Methods and applications, *Annu. Rep. NMR Spectrosc.* 93 (2018) 75–144, <https://doi.org/10.1016/bs.ammr.2017.08.003>.
- [22] M. Sattler, M. Maurer, J. Schleucher, C. Griesinger, A simultaneous ¹⁵N, ¹H- and ¹³C, ¹H-HSQC with sensitivity enhancement and a heteronuclear gradient echo, *J. Biomol. NMR* 5 (1995) 97–102, <https://doi.org/10.1007/BF00227475>.
- [23] P. Nolis, M. P  rez, T. Parella, Time-sharing evolution and sensitivity enhancements in 2D HSQC-TOCSY and HSQMBBC experiments, *Magn. Reson. Chem.* 44 (2006) 1031–1036, <https://doi.org/10.1002/mrc.1898>.
- [24] P. Nolis, M. P  rez-Trujillo, T. Parella, Multiple FID acquisition of complementary HMBBC data, *Angew. Chem. Int. Ed.* 46 (2007) 7495–7497, <https://doi.org/10.1002/anie.200702258>.
- [25] M. P  rez-Trujillo, P. Nolis, W. Bermel, T. Parella, Optimizing sensitivity and resolution in time-shared NMR experiments, *Magn. Reson. Chem.* 45 (2007) 325–329, <https://doi.org/10.1002/mrc.1973>.
- [26] T. Parella, P. Nolis, Time-shared NMR experiments, *Concepts Magn. Reson.* 36A (2010) 1–23, <https://doi.org/10.1002/cmr.a.20150>.
- [27] P. Nolis, K. Motiram-Corral, M. P  rez-Trujillo, T. Parella, Broadband homodecoupled time-shared ¹H-¹³C and ¹H-¹⁵N HSQC experiments, *J. Magn. Reson.* 298 (2019) 23–30, <https://doi.org/10.1016/j.jmr.2018.11.005>.
- [28] Ě. Kupĉe, R. Freeman, B.K. John, Parallel acquisition of two-dimensional NMR spectra of several nuclear species, *J. Am. Chem. Soc.* 128 (2006) 9606–9607, <https://doi.org/10.1021/ja0634876>.
- [29] Ě. Kupĉe, R. Freeman, Molecular structure from a single NMR experiment, *J. Am. Chem. Soc.* 130 (2008) 10788–10792, <https://doi.org/10.1021/ja8036492>.
- [30] Ě. Kupĉe, R. Freeman, Molecular structure from a single NMR sequence (fast-PANACEA), *J. Magn. Reson.* 206 (2010) 147–153, <https://doi.org/10.1016/j.jmr.2010.06.018>.
- [31] Ě. Kupĉe, R. Freeman, High-resolution NMR correlation experiments in a single measurement (HR-PANACEA), *Magn. Reson. Chem.* 48 (2010) 333–336, <https://doi.org/10.1002/mrc.2595>.
- [32] S.M. Pudakalakatti, A. Dubey, G. Jaipuria, U. Shubhashree, S.K. Adiga, D. Moskau, H.S. Atreya, A fast NMR method for resonance assignments: application to metabolomics, *J. Biomol. NMR* 58 (2014) 165–173, <https://doi.org/10.1007/s10858-014-9814-6>.
- [33] S.M. Pudakalakatti, A. Dubey, H.S. Atreya, Simultaneous acquisition of three NMR spectra in a single experiment for rapid resonance assignments in metabolomics, *J. Chem. Sci.* 127 (2015) 1091–1097, <https://doi.org/10.1007/s12039-015-0868-0>.
- [34] H. Kovacs, Ě. Kupĉe, Parallel NMR spectroscopy with simultaneous detection of ¹H and ¹⁹F nuclei, *Magn. Reson. Chem.* 54 (2016) 544–560, <https://doi.org/10.1002/mrc.4428>.
- [35] K. Motiram-Corral, M. P  rez-Trujillo, P. Nolis, T. Parella, Implementing one-shot multiple-FID acquisition into homonuclear and heteronuclear NMR experiments, *Chem. Commun.* 54 (2018) 13507–13510, <https://doi.org/10.1039/C8CC08065H>.
- [36] V.M.R. Kakita, K. Rachineni, M. Bopardikar, R.V. Hosur, NMR supersequences with real-time homonuclear broadband decoupling: Sequential acquisition of protein and small molecule spectra in a single experiment, *J. Magn. Reson.* 297 (2018) 108–112, <https://doi.org/10.1016/j.jmr.2018.10.013>.
- [37] T.M. Nagy, T. Gy  ngy  si, K.E. K  v  r, O.W. S  rensen, BANGO SEA XLOC/HMBC-H2OBC: complete heteronuclear correlation within minutes from one NMR pulse sequence, *Chem. Commun.* 55 (2019) 12208–12211, <https://doi.org/10.1039/C9CC06253J>.
- [38] P. Nolis, K. Motiram-Corral, M. P  rez-Trujillo, T. Parella, Interleaved dual NMR acquisition of equivalent transfer pathways in TOCSY and HSQC experiments, *ChemPhysChem* 20 (2019) 356–360, <https://doi.org/10.1002/cphc.201801034>.
- [39] P. Nolis, K. Motiram-Corral, M. P  rez-Trujillo, T. Parella, Simultaneous acquisition of two 2D HSQC spectra with different ¹³C spectral widths, *J. Magn. Reson.* 300 (2019) 1–7, <https://doi.org/10.1016/j.jmr.2019.01.004>.
- [40] P. Nolis, T. Parella, Practical aspects of the simultaneous collection of COSY and TOCSY spectra, *Magn. Reson. Chem.* 57 (2019) S85–S94, <https://doi.org/10.1002/mrc.4835>.
- [41] V.M.R. Kakita, R.V. Hosur, All-in-one NMR spectroscopy of small organic molecules: complete chemical shift assignment from a single NMR experiment, *RSC Adv.* 10 (2020) 21174–21179, <https://doi.org/10.1039/D0RA03417G>.
- [42] T.M. Nagy, K.E. K  v  r, O.W. S  rensen, Double and adiabatic BANGO for concatenating two NMR experiments relying on the same pool of magnetization, *J. Magn. Reson.* 316 (2020) 106767, <https://doi.org/10.1016/j.jmr.2020.106767>.
- [43] Ě. Kupĉe, K.R. Mote, A. Webb, P.K. Madhu, T.D.W. Claridge, Multiplexing experiments in NMR and multi-nuclear MRI, *Prog. Nucl. Magn. Reson. Spectrosc.* 124–125 (2021) 1–56, <https://doi.org/10.1016/j.pnmrs.2021.03.001>.
- [44] Ě. Kupĉe, T.D.W. Claridge, NOAH: NMR supersequences for small molecule analysis and structure elucidation, *Angew. Chem. Int. Ed.* 56 (2017) 11779–11783, <https://doi.org/10.1002/anie.201705506>.
- [45] Ě. Kupĉe, T.D.W. Claridge, Molecular structure from a single NMR supersequence, *Chem. Commun.* 54 (2018) 7139–7142, <https://doi.org/10.1039/C8CC03296C>.
- [46] T.D.W. Claridge, M. Mayzel, Ě. Kupĉe, Triplet NOAH supersequences optimised for small molecule structure characterisation, *Magn. Reson. Chem.* 57 (2019) 946–952, <https://doi.org/10.1002/mrc.4887>.
- [47] Ě. Kupĉe, T.D.W. Claridge, New NOAH modules for structure elucidation at natural isotopic abundance, *J. Magn. Reson.* 307 (2019) 106568, <https://doi.org/10.1016/j.jmr.2019.106568>.
- [48] Ě. Kupĉe, L. Frydman, A.G. Webb, J.R.J. Yong, T.D.W. Claridge, Parallel nuclear magnetic resonance spectroscopy, *Nat. Rev. Methods Primers* 1 (2021) 27, <https://doi.org/10.1038/s43586-021-00024-3>.
- [49] T.D.W. Claridge, *High-Resolution NMR Techniques in Organic Chemistry*, 3rd Edition, Elsevier, Amsterdam, 2016.
- [50] J. Cavanagh, W.J. Fairbrother, A.G. Palmer III, W. Rance, N.J. Skelton, *Protein NMR Spectroscopy: Principles and Practice*, 2nd Edition, Academic Press, Burlington, MA, 2007.
- [51] J.R. Garbow, D.P. Weitekamp, A. Pines, Bilinear rotation decoupling of homonuclear scalar interactions, *Chem. Phys. Lett.* 93 (1982) 504–509, [https://doi.org/10.1016/0009-2614\(82\)83229-6](https://doi.org/10.1016/0009-2614(82)83229-6).
- [52] S. Wimpey, R. Freeman, An excitation sequence which discriminates between direct and long-range CH coupling, *J. Magn. Reson.* 58 (1984) 348–353, [https://doi.org/10.1016/0022-2364\(84\)90227-0](https://doi.org/10.1016/0022-2364(84)90227-0).
- [53] D. Uhrin, T. Liptaj, K.E. K  v  r, Modified BIRD pulses and design of heteronuclear pulse sequences, *J. Magn. Reson.* 101 (1993) 41–46, <https://doi.org/10.1006/jmra.1993.1005>.
- [54] O.W. S  rensen, Selective rotations using non-selective pulses and heteronuclear couplings, *Bull. Magn. Reson.* 16 (1994) 49–53.
- [55] J. Briand, O.W. S  rensen, A novel pulse sequence element for selective and independent rotations with arbitrary flip angles and phases for I and I(S) spin systems, *J. Magn. Reson.* 125 (1997) 202–206, <https://doi.org/10.1006/jmre.1996.1095>.
- [56] J. Briand, O.W. S  rensen, Simultaneous and independent rotations with arbitrary flip angles and phases for I, I_{Sx}, and I_{Sy} spin systems, *J. Magn. Reson.* 135 (1998) 44–49, <https://doi.org/10.1006/jmre.1998.1556>.
- [57] J. Orts, A.D. Gossert, Structure determination of protein–ligand complexes by NMR in solution, *Methods* 138–139 (2018) 3–25, <https://doi.org/10.1016/j.ymeth.2018.01.019>.
- [58] A.G. Palmer, J. Cavanagh, P.E. Wright, M. Rance, Sensitivity improvement in proton-detected two-dimensional heteronuclear correlation NMR spectroscopy, *J. Magn. Reson.* 93 (1991) 151–170, [https://doi.org/10.1016/0022-2364\(91\)90036-S](https://doi.org/10.1016/0022-2364(91)90036-S).
- [59] L. Kay, P. Keifer, T. Saarinen, Pure absorption gradient enhanced heteronuclear single quantum correlation spectroscopy with improved sensitivity, *J. Am. Chem. Soc.* 114 (1992) 10663–10665, <https://doi.org/10.1021/ja00052a088>.
- [60] J. Cavanagh, M. Rance, Sensitivity improvement in isotropic mixing (TOCSY) experiments, *J. Magn. Reson.* 88 (1990) 72–85, [https://doi.org/10.1016/0022-2364\(90\)90109-M](https://doi.org/10.1016/0022-2364(90)90109-M).
- [61] J. Cavanagh, M. Rance, Sensitivity-enhanced NMR techniques for the study of biomolecules, *Annu. Rep. NMR Spectrosc.* 27 (1993) 1–58, [https://doi.org/10.1016/S0066-4103\(08\)60264-1](https://doi.org/10.1016/S0066-4103(08)60264-1).

- [62] M.R.M. Koos, G. Kummerl  we, L. Kaltschnee, C.M. Thiele, B. Luy, CLIP-COSY: A clean in-phase experiment for the rapid acquisition of COSY-type correlations, *Angew. Chem. Int. Ed.* 55 (2016) 7655–7659, <https://doi.org/10.1002/anie.201510938>.
- [63] J. Schleucher, M. Schwendinger, M. Sattler, P. Schmidt, O. Schedletsky, S.J. Glaser, O.W. S  rensen, C. Griesinger, A general enhancement scheme in heteronuclear multidimensional NMR employing pulsed field gradients, *J. Biomol. NMR* 4 (1994) 301–306, <https://doi.org/10.1007/BF00175254>.
- [64] G. Kontaxis, J. Stonehouse, E.D. Laue, J. Keeler, The sensitivity of experiments which use gradient pulses for coherence-pathway selection, *J. Magn. Reson.* 111 (1994) 70–76, <https://doi.org/10.1006/jmra.1994.1227>.
- [65] M.J. Thrippleton, J. Keeler, Elimination of zero-quantum interference in two-dimensional NMR spectra, *Angew. Chem. Int. Ed.* 42 (2003) 3938–3941, <https://doi.org/10.1002/anie.200351947>.
- [66] A.L. Hansen, Ě. Kupĉe, D.-W. Li, L. Br  schweiler-Li, C. Wang, R. Br  schweiler, 2D NMR-based metabolomics with HSQC/TOCSY NOAH supersequences, *Anal. Chem.* 93 (2021) 6112–6119, <https://doi.org/10.1021/acs.analchem.0c05205>.
- [67] T. Parella, F. S  nchez-Ferrando, A. Virgili, Improved sensitivity in gradient-based 1D and 2D multiplicity-edited HSQC experiments, *J. Magn. Reson.* 126 (1997) 274–277, <https://doi.org/10.1006/jmre.1997.1164>.
- [68] D. Tufts, R. Kumaresan, Singular value decomposition and improved frequency estimation using linear prediction, *IEEE Trans. Acoust., Speech, Signal Process.* 30 (1982) 671–675, <https://doi.org/10.1109/TASSP.1982.1163927>.
- [69] J.J. Led, H. Gesmar, Application of the linear prediction method to NMR spectroscopy, *Chem. Rev.* 91 (1991) 1413–1426, <https://doi.org/10.1021/cr00007a007>.
- [70] P. Koehl, Linear prediction spectral analysis of NMR data, *Prog. Nucl. Magn. Reson. Spectrosc.* 34 (1999) 257–299, [https://doi.org/10.1016/S0079-6565\(99\)00002-3](https://doi.org/10.1016/S0079-6565(99)00002-3).
- [71] D.L. Donoho, I.M. Johnstone, A.S. Stern, J.C. Hoch, Does the maximum entropy method improve sensitivity?, *Proc. Natl. Acad. Sci. U.S.A.* 87 (1990) 5066–5068, <https://doi.org/10.1073/pnas.87.13.5066>.
- [72] A.S. Stern, K.-B. Li, J.C. Hoch, Modern spectrum analysis in multidimensional NMR spectroscopy: comparison of linear-prediction extrapolation and maximum-entropy reconstruction, *J. Am. Chem. Soc.* 124 (2002) 1982–1993, <https://doi.org/10.1021/ja011669o>.
- [73] M.R. Palmer, C.L. Suiter, G.E. Henry, J. Rovnyak, J.C. Hoch, T. Polenova, D. Rovnyak, Sensitivity of nonuniform sampling NMR, *J. Phys. Chem. B* 119 (2015) 6502–6515, <https://doi.org/10.1021/jp5126415>.
- [74] K. Kazimierczuk, J. Stanek, A. Zawadzka-Kazimierczuk, W. Kozmi  nski, Random sampling in multidimensional NMR spectroscopy, *Prog. Nucl. Magn. Reson. Spectrosc.* 57 (2010) 420–434, <https://doi.org/10.1016/j.pnmrs.2010.07.002>.
- [75] M. Mobli, J.C. Hoch, Nonuniform sampling and non-Fourier signal processing methods in multidimensional NMR, *Prog. Nucl. Magn. Reson. Spectrosc.* 83 (2014) 21–41, <https://doi.org/10.1016/j.pnmrs.2014.09.002>.
- [76] K. Kazimierczuk, V. Orekhov, Non-uniform sampling: post-Fourier era of NMR data collection and processing, *Magn. Reson. Chem.* 53 (2015) 921–926, <https://doi.org/10.1002/mrc.4284>.
- [77] D. Go  łowicz, P. Kasprzak, V. Orekhov, K. Kazimierczuk, Fast time-resolved NMR with non-uniform sampling, *Prog. Nucl. Magn. Reson. Spectrosc.* 116 (2020) 40–55, <https://doi.org/10.1016/j.pnmrs.2019.09.003>.